
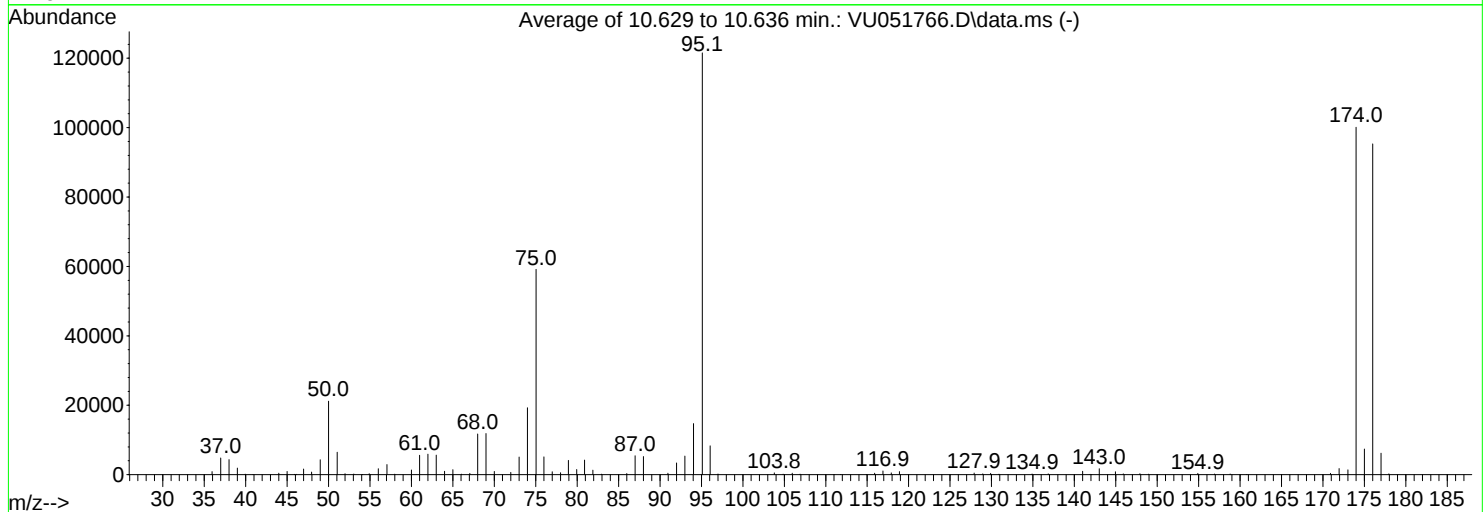


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110722\
Data File : VU051766.D
Acq On : 07 Nov 2022 08:38
Operator : JC/MD
Sample : BFB141
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB141

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Title : VOC Analysis
Last Update : Tue Nov 08 00:38:03 2022

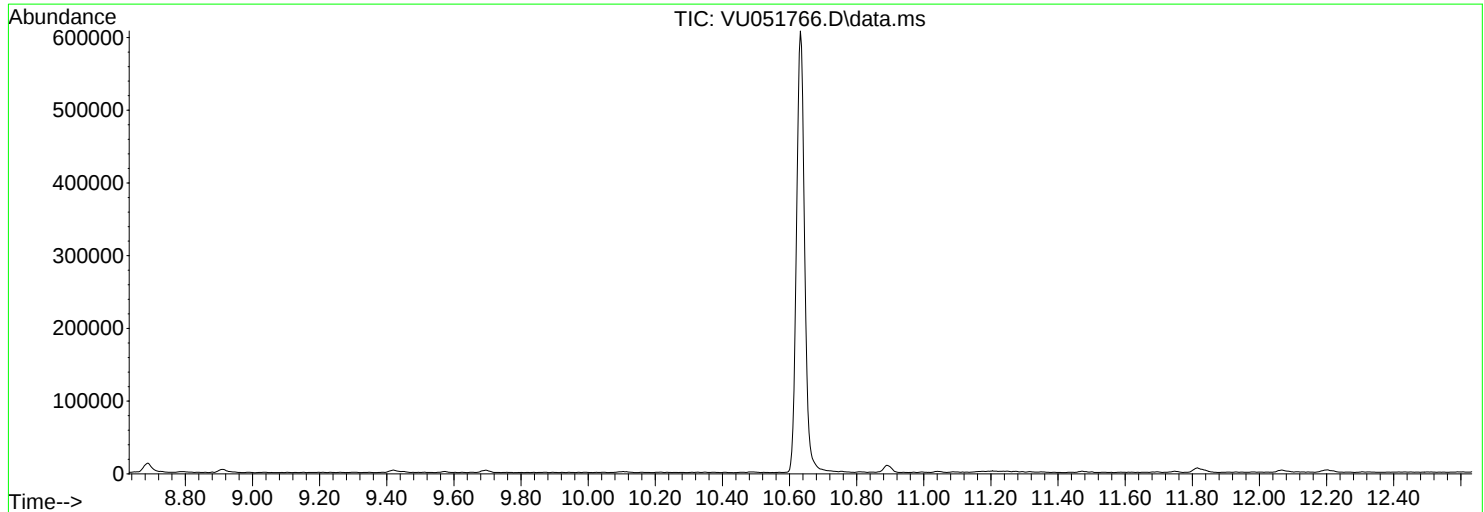

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	21144	PASS
75	95	30	80	48.7	59149	PASS
95	95	100	100	100.0	121552	PASS
96	95	5	9	6.8	8304	PASS
173	174	0.00	2	1.4	1395	PASS
174	95	50	120	82.4	100101	PASS
175	174	5	9	7.4	7362	PASS
176	174	95	101	95.2	95317	PASS
177	176	5	9	6.5	6178	PASS

Scan 2876 (10.587 min): VU051766.D\data.ms
BFB141

m/z	Abundance
40.00	1665.0
44.00	538.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
35.90	899.0
37.00	4794.0
38.00	4370.0
39.00	1989.0
39.90	1862.0
44.00	873.0
45.00	1015.0
45.90	222.0
47.00	1452.0
47.90	780.0
49.00	4252.0
50.00	21056.0
51.10	6497.0
52.00	291.0
53.00	221.0
54.10	104.0
54.90	299.0
56.00	1737.0
57.00	2914.0
58.00	122.0
60.00	1281.0
61.00	5175.0
62.00	5922.0
63.00	5687.0
64.00	1063.0
65.00	1387.0
66.00	151.0
67.00	425.0
68.00	11474.0
69.00	12158.0
70.00	889.0
72.00	615.0
73.00	4911.0
74.00	19184.0
75.00	57984.0
76.00	5272.0
77.00	784.0
78.00	552.0
78.90	3977.0
79.90	1421.0
80.90	4063.0
81.90	1227.0
82.90	103.0
86.00	309.0
87.00	5309.0
88.00	5338.0
90.90	352.0
92.00	3407.0
93.00	5051.0
94.10	14375.0
95.10	118816.0
96.00	7996.0
97.00	165.0
103.80	521.0
105.00	140.0
105.90	400.0
106.90	142.0
111.00	104.0
111.80	102.0
115.90	411.0
116.90	1006.0
117.90	433.0
118.90	819.0
127.90	430.0
129.00	195.0
129.90	405.0
131.00	110.0
134.90	198.0
136.80	211.0
141.00	932.0
141.90	127.0
143.00	1506.0
144.90	964.0
145.80	220.0
147.90	320.0
148.90	119.0
154.90	401.0
156.90	150.0
158.80	173.0
160.80	100.0
170.90	423.0
172.00	1726.0
173.00	1342.0
174.00	96464.0
175.00	7311.0
176.00	91784.0
177.00	6168.0
178.00	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
35.90	914.0
37.00	4916.0
38.00	4436.0
39.00	1896.0
39.90	1797.0
44.00	961.0
45.00	945.0
46.10	173.0
47.00	1660.0
47.90	787.0
49.00	4434.0
50.00	21872.0
51.00	6660.0
52.00	284.0
53.00	186.0
54.90	312.0
56.00	1790.0
57.10	2974.0
58.00	138.0
60.00	1448.0
61.00	5743.0
62.00	6152.0
63.00	5849.0
64.00	979.0
65.00	1493.0
66.00	135.0
67.00	393.0
68.00	11975.0
69.00	12140.0
70.00	956.0
72.00	685.0
73.00	5164.0
74.00	19824.0
75.10	60960.0
76.00	5286.0
77.00	870.0
78.00	580.0
79.00	4203.0
79.90	1505.0
80.90	4331.0
81.90	1333.0
82.90	127.0
86.00	349.0
87.00	5614.0
88.00	5306.0
90.90	424.0
92.00	3420.0
93.00	5458.0
94.10	15129.0
95.10	125064.0
96.10	8617.0
97.00	208.0
103.80	521.0
104.80	148.0
105.90	401.0
106.90	116.0
111.80	112.0
115.90	421.0
116.90	1128.0
117.90	480.0
118.90	877.0
127.90	454.0
128.90	229.0
129.90	395.0
130.90	142.0
134.90	201.0
136.90	259.0
141.00	974.0
141.90	125.0
143.00	1727.0
145.00	862.0
145.90	262.0
147.90	311.0
148.90	133.0
154.90	388.0
156.90	198.0
158.80	219.0
170.90	406.0
172.00	1805.0
173.00	1432.0
174.00	103224.0
175.00	7566.0
176.00	97912.0
177.00	6381.0
177.90	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
36.00	891.0
37.00	4654.0
38.00	4141.0
39.00	1826.0
40.00	1701.0
40.90	112.0
44.00	1000.0
45.00	871.0
46.10	149.0
47.00	1705.0
48.00	679.0
49.00	4197.0
50.00	20504.0
51.00	6170.0
52.00	299.0
53.10	145.0
54.90	293.0
56.00	1600.0
57.10	2788.0
58.00	151.0
60.00	1333.0
61.00	5808.0
62.00	5686.0
63.00	5314.0
64.00	815.0
65.00	1470.0
66.10	143.0
67.10	310.0
68.00	11733.0
69.00	11227.0
70.00	918.0
72.00	630.0
73.00	5127.0
74.00	18824.0
75.00	58504.0
76.00	4803.0
77.00	883.0
78.00	601.0
79.00	4142.0
80.00	1441.0
80.90	4273.0
81.90	1283.0
83.00	140.0
86.00	297.0
87.00	5428.0
88.00	5036.0
91.00	454.0
92.00	3268.0
93.00	5576.0
94.00	14591.0
95.10	120776.0
96.10	8298.0
97.00	228.0
103.80	455.0
104.80	141.0
106.00	419.0
106.90	104.0
114.90	136.0
115.90	390.0
116.90	1045.0
117.90	552.0
118.90	878.0
127.90	459.0
128.90	238.0
129.90	355.0
130.80	135.0
134.90	208.0
136.90	244.0
141.00	948.0
142.10	130.0
143.00	1905.0
145.00	704.0
146.00	270.0
147.90	264.0
149.00	111.0
154.90	300.0
156.90	201.0
158.80	181.0
170.90	351.0
171.90	1731.0
173.00	1410.0
174.00	100616.0
175.00	7209.0
176.00	96256.0
177.00	5984.0
177.90	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141