


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110723\
Data File : VU056087.D
Acq On : 07 Nov 2023 07:55
Operator : MD/SY
Sample : BFB067
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB067

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 08 00:38:11 2023

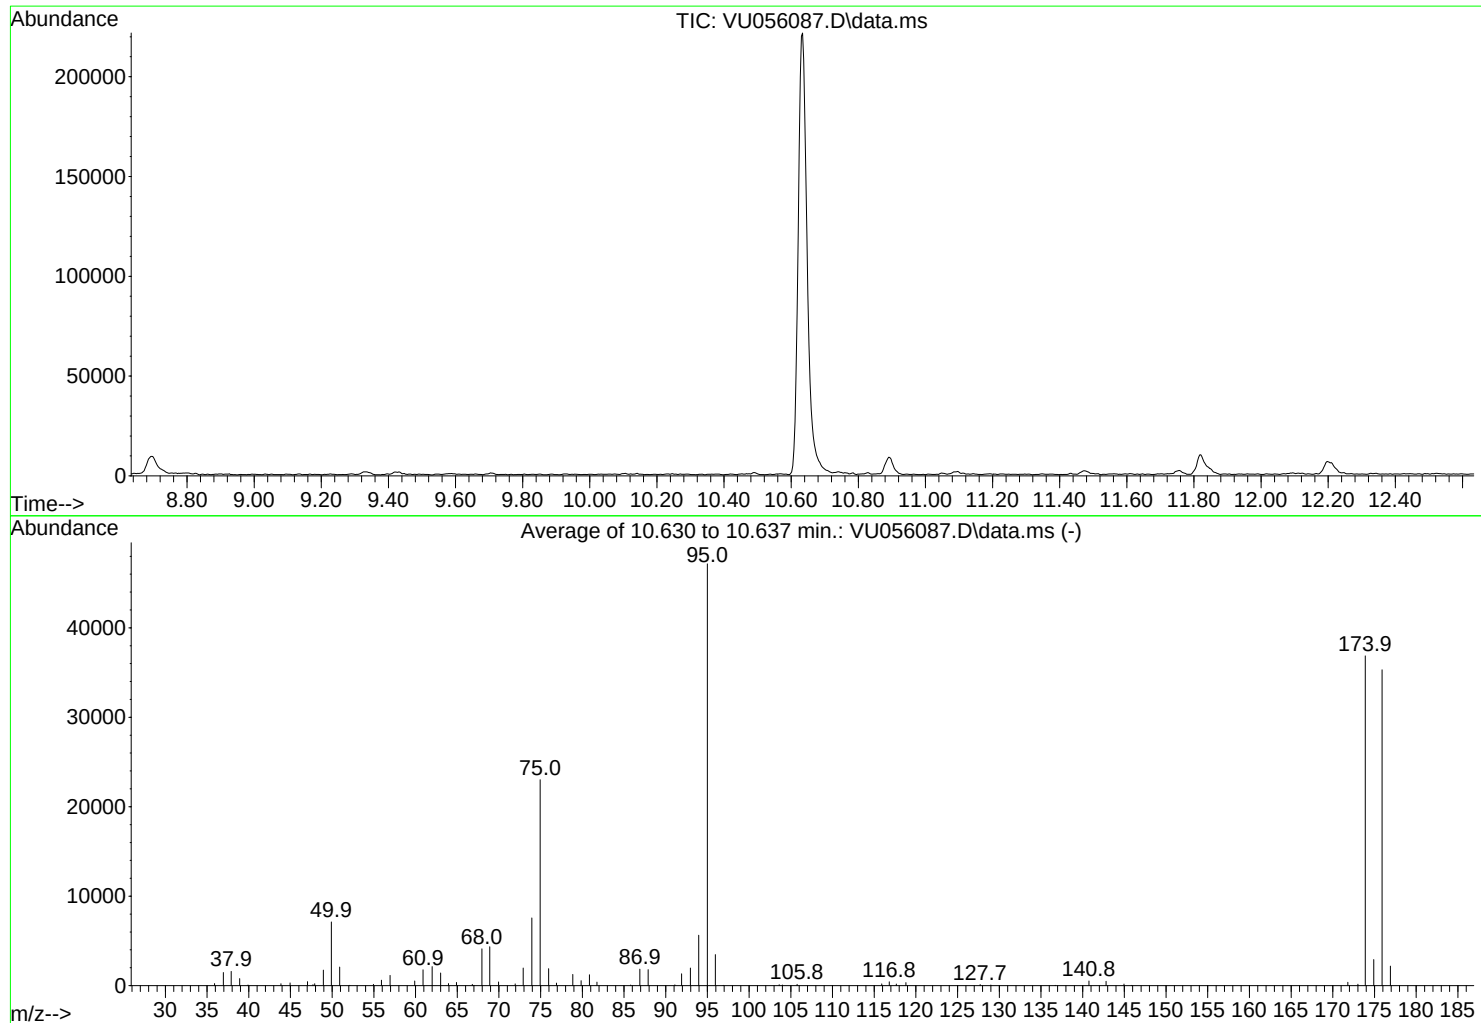

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	7126	PASS
75	95	30	80	48.8	23019	PASS
95	95	100	100	100.0	47155	PASS
96	95	5	9	7.4	3473	PASS
173	174	0.00	2	0.4	160	PASS
174	95	50	120	78.2	36867	PASS
175	174	5	9	7.9	2915	PASS
176	174	95	101	95.8	35304	PASS
177	176	5	9	6.2	2184	PASS

m/z	Abundance
39.80	276.0
43.80	462.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	261.0
36.90	1442.0
37.90	1672.0
38.90	845.0
39.70	256.0
43.90	684.0
44.90	364.0
47.00	486.0
47.70	308.0
49.00	1936.0
49.90	7471.0
50.90	2248.0
52.10	118.0
55.00	156.0
55.90	677.0
57.00	1251.0
59.90	446.0
60.90	1892.0
62.00	2267.0
63.00	1401.0
63.90	210.0
65.00	302.0
66.80	231.0
68.00	4180.0
68.90	4574.0
69.90	391.0
71.90	160.0
72.90	1982.0
74.00	7577.0
74.90	23408.0
76.00	2004.0
76.90	251.0
78.80	1298.0
79.80	573.0
80.80	1266.0
81.70	322.0
86.90	2017.0
87.90	1829.0
91.90	1316.0
93.00	1965.0
94.00	5620.0
95.00	47808.0
96.00	3439.0
96.90	109.0
104.00	193.0
105.80	133.0
115.90	178.0
116.80	430.0
117.60	111.0
118.80	319.0
127.70	106.0
129.00	114.0
140.70	426.0
142.80	462.0
144.90	160.0
171.80	364.0
173.00	481.0
173.90	37088.0
174.90	2890.0
175.90	35528.0
176.90	2220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	232.0
36.90	1532.0
37.90	1612.0
38.90	842.0
39.70	225.0
43.90	688.0
45.00	292.0
47.10	419.0
47.90	301.0
48.90	1779.0
49.90	7219.0
50.90	2049.0
55.00	162.0
55.90	610.0
56.90	1147.0
59.90	540.0
60.90	1780.0
62.00	2190.0
63.00	1464.0
64.00	245.0
64.90	378.0
66.80	186.0
67.90	4260.0
68.90	4522.0
69.90	429.0
72.00	209.0
72.90	2019.0
73.90	7688.0
75.00	23536.0
76.00	1913.0
76.90	288.0
78.80	1239.0
79.80	580.0
80.90	1245.0
81.80	399.0
85.80	113.0
86.90	1814.0
87.90	1847.0
91.10	131.0
91.90	1369.0
92.90	2008.0
93.90	5823.0
95.00	48192.0
96.00	3598.0
103.60	178.0
105.80	143.0
115.90	191.0
116.80	467.0
117.70	185.0
118.80	351.0
127.70	122.0
129.00	112.0
140.80	574.0
142.80	506.0
145.00	188.0
171.80	408.0
173.90	37856.0
174.90	3019.0
175.90	36280.0
176.90	2168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	210.0
37.00	1433.0
37.90	1519.0
38.90	691.0
39.90	219.0
43.90	659.0
45.00	246.0
47.10	428.0
47.90	329.0
48.90	1509.0
49.90	6688.0
50.90	1909.0
54.90	132.0
55.90	530.0
56.90	1019.0
59.90	598.0
60.90	1650.0
62.00	1959.0
63.00	1378.0
64.00	267.0
64.80	370.0
67.00	113.0
67.90	3912.0
68.90	3976.0
70.00	413.0
71.90	220.0
72.90	1883.0
73.90	7409.0
75.00	22112.0
75.90	1780.0
76.90	298.0
78.90	1198.0
79.90	520.0
80.90	1123.0
81.80	473.0
85.80	101.0
86.90	1722.0
87.90	1721.0
91.10	130.0
91.90	1297.0
92.90	1946.0
93.90	5448.0
95.00	45464.0
95.90	3383.0
103.60	162.0
105.70	157.0
115.90	218.0
116.80	368.0
117.70	232.0
118.80	329.0
127.70	140.0
136.70	103.0
140.80	571.0
142.80	495.0
145.00	198.0
145.90	116.0
171.80	383.0
173.90	35656.0
174.90	2836.0
175.90	34104.0
176.90	2163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067