


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU110818\  
Data File : VU028011.D  
Acq On : 08 Nov 2018 09:03  
Operator : MD/SY  
Sample : BFB  
Misc : 5.0mL/MSVOA U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U110218W.M  
Title : SW846 8260  
Last Update : Fri Nov 02 02:28:20 2018

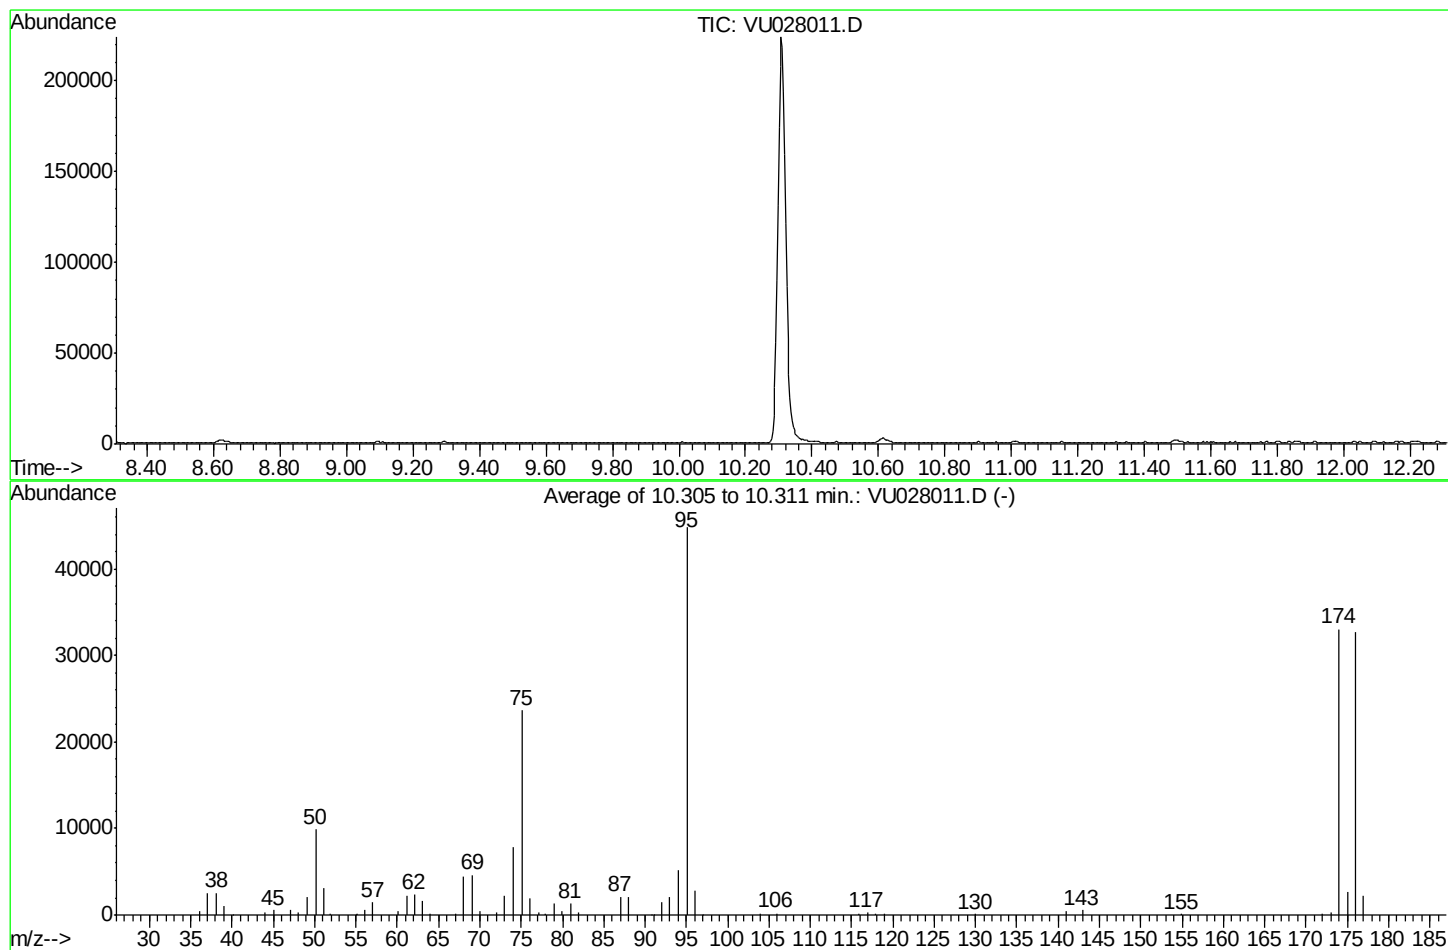

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.1      | 9912    | PASS             |
| 75          | 95           | 30           | 60           | 52.7      | 23613   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 44824   | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 2817    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 291     | PASS             |
| 174         | 95           | 50           | 100          | 73.7      | 33032   | PASS             |
| 175         | 174          | 5            | 9            | 7.9       | 2605    | PASS             |
| 176         | 174          | 95           | 101          | 99.2      | 32757   | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 2253    | PASS             |