
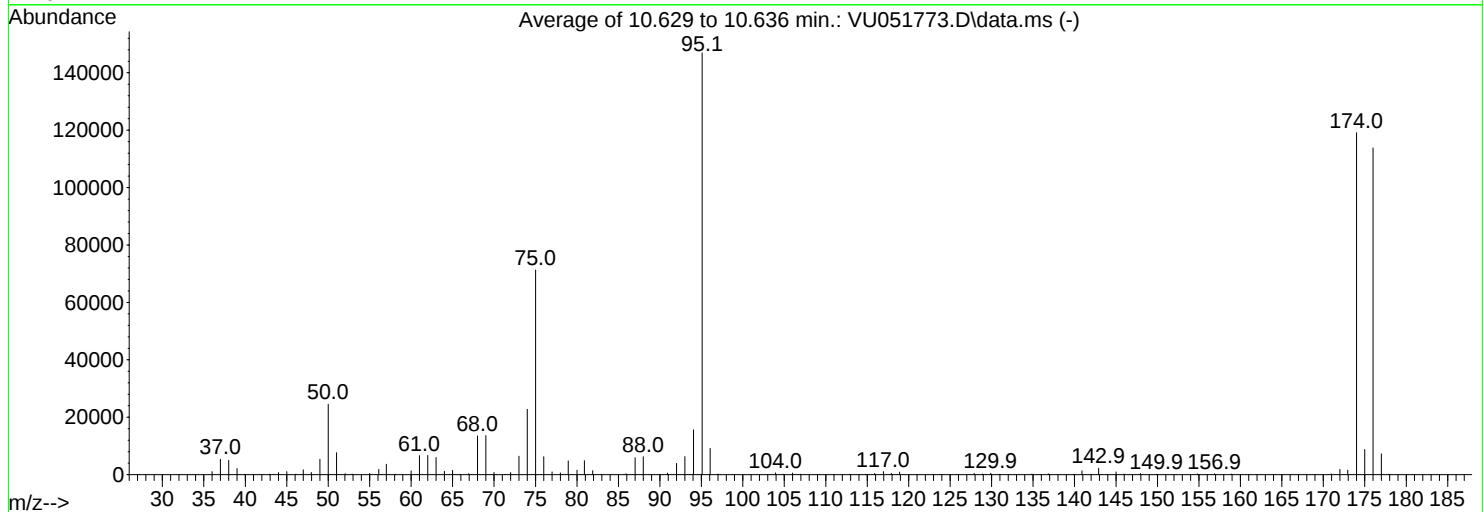


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110822\
 Data File : VU051773.D
 Acq On : 08 Nov 2022 09:02
 Operator : JC/MD
 Sample : BFB165
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB165

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 08 23:59:15 2022

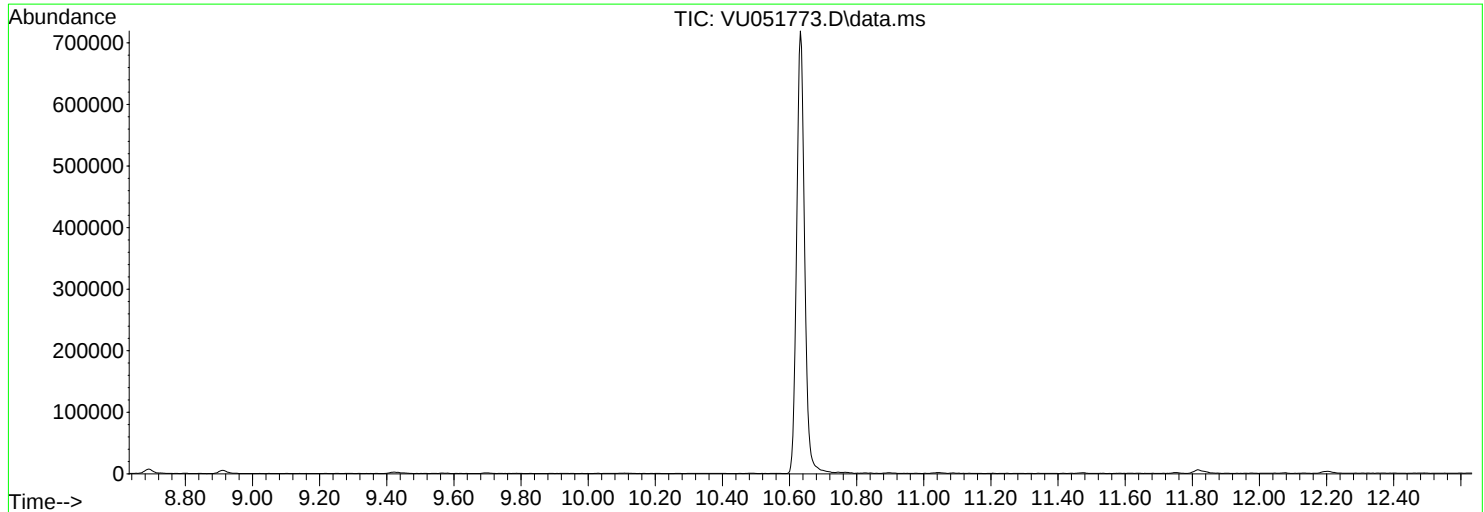

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	24512	PASS
75	95	30	80	48.5	71307	PASS
95	95	100	100	100.0	146944	PASS
96	95	5	9	6.2	9174	PASS
173	174	0.00	2	1.3	1586	PASS
174	95	50	120	81.1	119125	PASS
175	174	5	9	7.4	8776	PASS
176	174	95	101	95.6	113827	PASS
177	176	5	9	6.4	7267	PASS

m/z	Abundance
39.90	169.0
44.00	338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
36.00	1045.0
37.00	5294.0
38.00	5198.0
39.00	2245.0
39.90	262.0
42.90	145.0
44.00	1198.0
45.00	1068.0
46.10	108.0
47.00	1626.0
48.00	702.0
49.00	5391.0
50.00	24256.0
51.00	7446.0
52.10	396.0
52.90	196.0
55.00	387.0
56.10	1902.0
57.00	3491.0
60.00	1163.0
61.00	6708.0
62.00	6438.0
63.00	6045.0
64.00	1228.0
65.00	1398.0
65.90	126.0
67.00	352.0
68.00	13277.0
69.00	13377.0
70.00	849.0
72.00	766.0
73.00	6155.0
74.00	22536.0
75.00	70152.0
76.00	6463.0
77.00	900.0
78.00	635.0
78.90	4684.0
80.00	1527.0
80.90	4831.0
81.90	1425.0
82.90	125.0
85.90	365.0
87.00	6088.0
88.00	6171.0
90.90	549.0
92.00	4044.0
93.00	6269.0
94.00	15116.0
95.10	144000.0
96.00	9179.0
97.00	208.0
103.90	563.0
104.90	205.0
106.00	627.0
107.00	160.0
111.00	126.0
112.80	156.0
115.90	519.0
117.00	1026.0
117.90	427.0
118.90	875.0
127.90	465.0
128.90	249.0
129.90	537.0
130.90	122.0
134.90	185.0
135.90	109.0
136.80	210.0
139.90	104.0
140.90	1289.0
142.00	191.0
142.90	2181.0
143.90	131.0
145.00	1031.0
146.00	202.0
147.90	450.0
149.00	118.0
149.90	138.0
154.90	257.0
156.90	336.0
158.90	204.0
161.00	149.0
171.00	323.0
172.00	1826.0
173.00	1683.0
174.00	114056.0
175.00	8416.0
176.00	108424.0
177.00	7321.0
177.90	220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
36.00	1038.0
37.00	5484.0
38.00	5145.0
39.00	2178.0
39.90	225.0
42.90	170.0
44.00	1105.0
45.00	1063.0
46.10	166.0
47.00	1716.0
47.90	791.0
49.00	5511.0
50.00	25288.0
51.00	7830.0
52.00	361.0
52.90	198.0
55.00	392.0
56.10	1894.0
57.00	3743.0
58.10	122.0
60.00	1363.0
61.00	6891.0
62.00	6838.0
63.00	6153.0
64.00	1238.0
65.00	1576.0
65.80	124.0
66.90	379.0
68.00	13915.0
69.00	14168.0
70.00	832.0
72.00	819.0
73.00	6705.0
74.00	23600.0
75.00	73312.0
76.00	6432.0
77.00	956.0
78.00	604.0
78.90	4835.0
80.00	1655.0
80.90	4989.0
81.90	1414.0
82.90	138.0
85.90	379.0
87.00	6028.0
88.00	6425.0
90.90	557.0
92.00	4026.0
93.00	6482.0
94.10	16015.0
95.10	151616.0
96.00	9454.0
97.00	253.0
103.90	666.0
104.90	184.0
106.00	585.0
106.90	145.0
111.00	142.0
112.80	146.0
114.80	134.0
115.90	471.0
116.90	1116.0
117.90	479.0
118.90	940.0
123.80	125.0
127.90	476.0
128.90	232.0
129.90	535.0
130.90	149.0
134.80	245.0
136.80	279.0
139.80	108.0
140.90	1409.0
142.00	136.0
142.90	2278.0
144.00	101.0
145.00	998.0
146.00	231.0
147.90	389.0
149.90	141.0
154.80	285.0
156.90	331.0
158.90	230.0
161.00	133.0
171.00	286.0
172.00	1866.0
172.90	1664.0
174.00	122920.0
175.00	9013.0
176.00	117384.0
177.00	7476.0
177.90	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
36.00	1038.0
37.00	5280.0
38.00	4612.0
39.00	2013.0
40.00	236.0
42.90	122.0
44.00	967.0
45.00	1003.0
46.10	189.0
47.00	1701.0
48.00	833.0
49.00	5151.0
50.00	23992.0
51.00	7577.0
52.00	340.0
52.90	182.0
55.00	330.0
56.10	1788.0
57.00	3671.0
58.10	154.0
60.00	1474.0
61.00	6342.0
62.00	6775.0
63.00	5767.0
64.00	1068.0
65.00	1619.0
65.90	114.0
66.90	362.0
68.00	13363.0
69.00	13329.0
70.00	763.0
71.30	110.0
72.00	675.0
73.00	6433.0
74.00	22152.0
75.00	70456.0
76.00	5839.0
77.00	978.0
78.00	548.0
79.00	4794.0
80.00	1577.0
80.90	4742.0
81.90	1338.0
82.90	131.0
85.90	356.0
87.00	5702.0
88.00	6092.0
90.90	534.0
92.00	3735.0
93.00	6143.0
94.10	15668.0
95.10	145216.0
96.10	8889.0
97.00	220.0
104.00	653.0
105.00	197.0
106.00	538.0
106.90	153.0
111.00	136.0
112.80	126.0
114.80	157.0
115.90	420.0
116.90	1053.0
117.90	481.0
118.90	902.0
123.80	113.0
127.90	447.0
128.90	199.0
129.90	493.0
130.90	185.0
134.90	252.0
136.90	304.0
139.80	116.0
140.90	1291.0
141.90	116.0
142.90	2207.0
145.00	790.0
145.90	239.0
148.00	344.0
149.90	127.0
154.90	298.0
156.90	315.0
158.90	226.0
161.00	111.0
170.90	281.0
172.00	1766.0
172.90	1410.0
174.00	120400.0
175.00	8900.0
176.00	115672.0
177.00	7005.0
177.90	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165