

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110823\
 Data File : VU056125.D
 Acq On : 08 Nov 2023 15:40
 Operator : MD/SY
 Sample : 05297-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Quant Time: Nov 08 20:53:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 08 20:49:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	364002	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	367780	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	159822	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	119538	5.291	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.800%	
7) Chloroethane-d5	1.907	69	95737	6.244	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	124.800%	
11) 1,1-Dichloroethene-d2	2.563	65	52419	5.266	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	105.400%	
20) 2-Butanone-d5	4.621	46	243636	65.730	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	131.460%#	
24) Chloroform-d	5.055	84	238568	5.547	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	111.000%	
26) 1,2-Dichloroethane-d4	5.695	65	113088	5.972	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	119.400%	
32) Benzene-d6	5.721	84	484606	5.486	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.800%	
36) 1,2-Dichloropropane-d6	6.685	67	148389	5.707	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	114.200%	
41) Toluene-d8	7.894	98	408526	5.047	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
43) trans-1,3-Dichloroprop...	8.177	79	51064	5.138	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	102.800%	
46) 2-Hexanone-d5	8.631	63	188808	57.959	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	115.920%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	106962	5.764	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	115.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152	145297	5.895	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	118.000%	
Target Compounds					Qvalue	
13) Acetone	2.628	43	40313	14.747	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110823\
Data File : VU056125.D
Acq On : 08 Nov 2023 15:40
Operator : MD/SY
Sample : 05297-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Time: Nov 08 20:53:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 08 20:49:31 2023
Response via : Initial Calibration

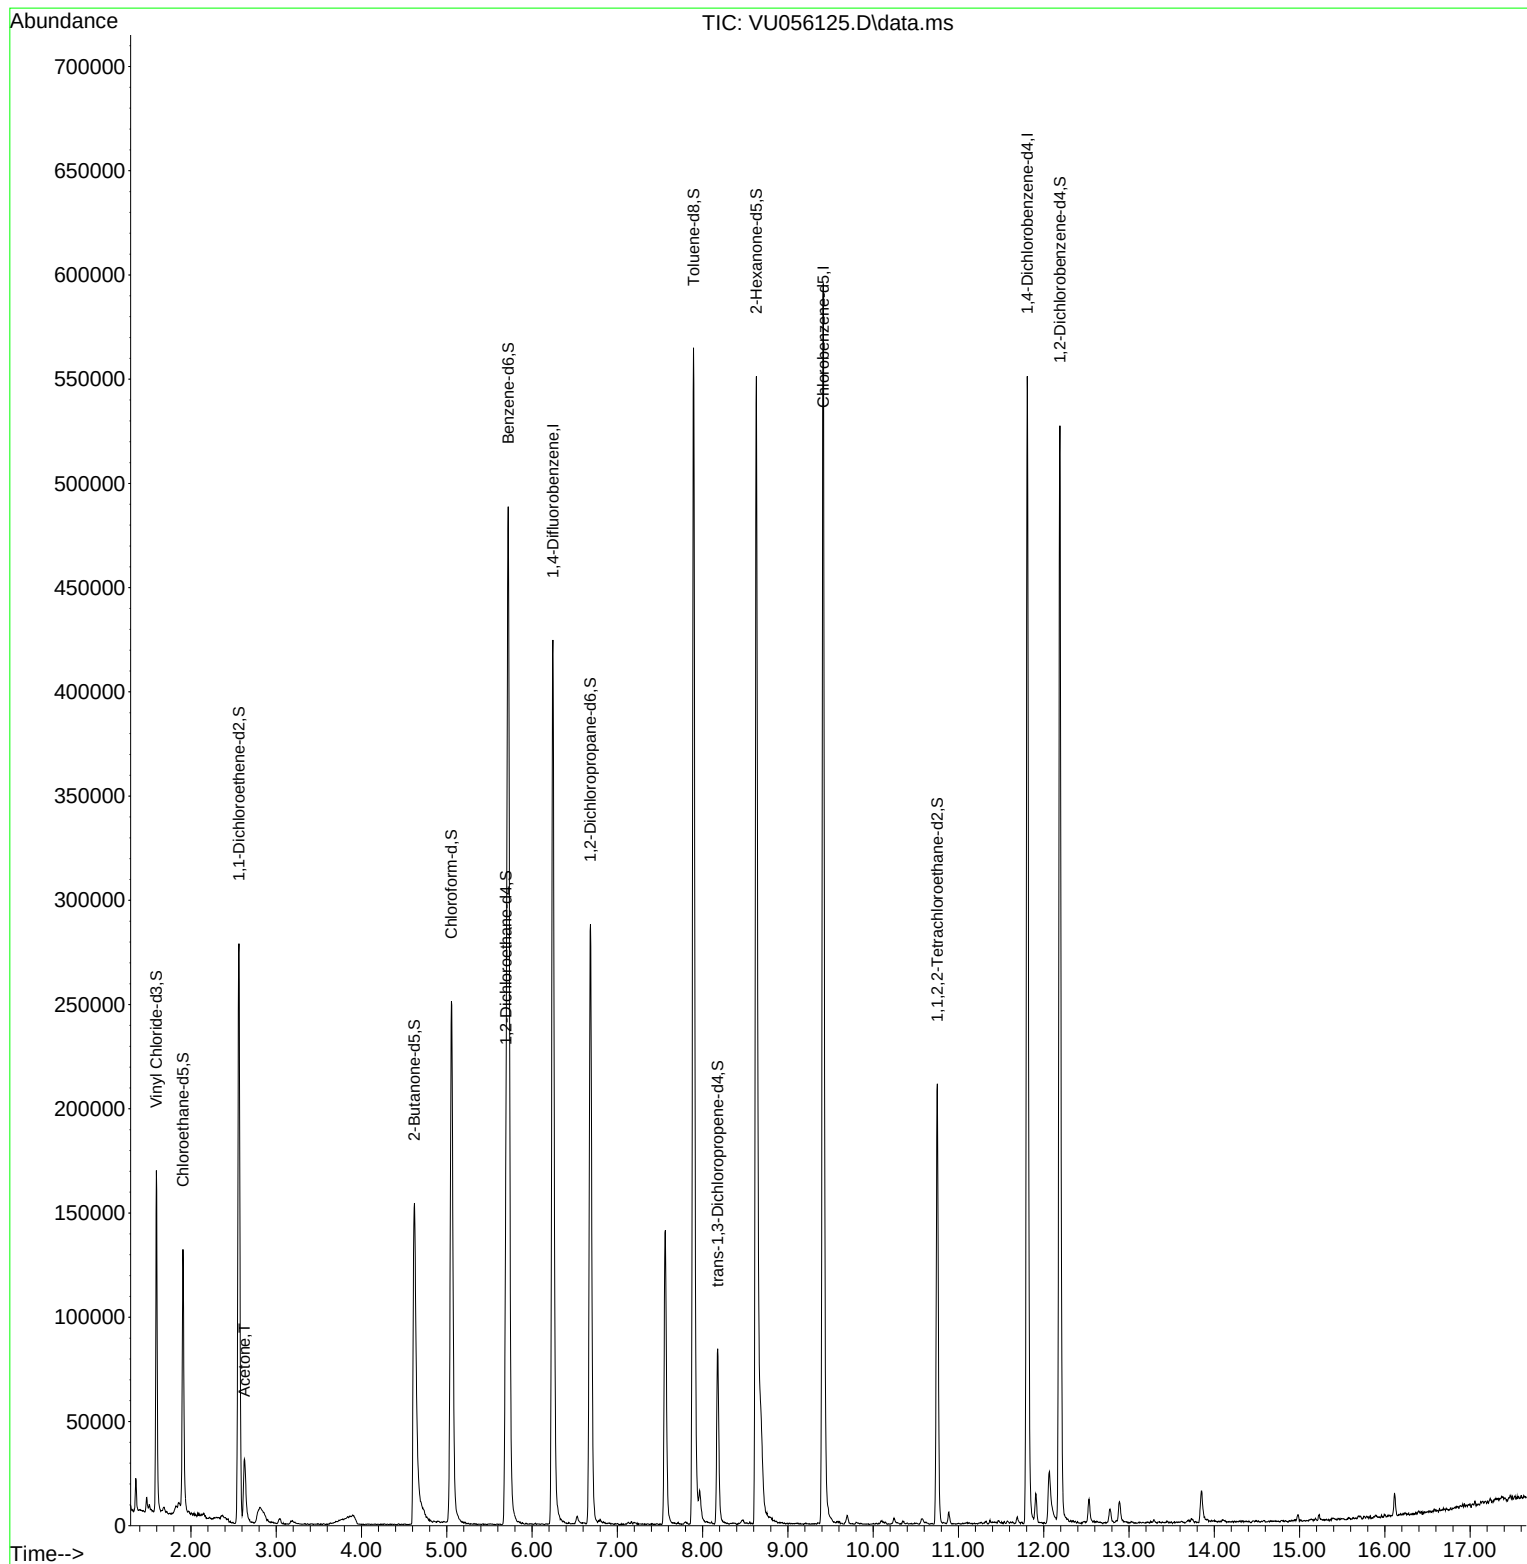

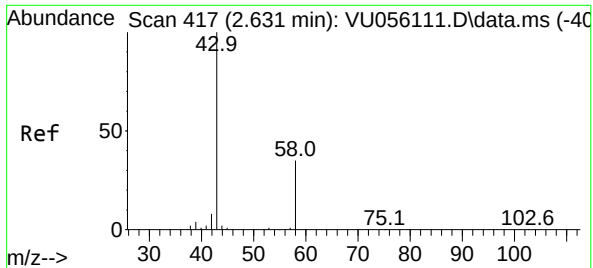

#13
 Acetone
 Concen: 14.747 ug/L
 RT: 2.628 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU056125.D
 Acq: 08 Nov 2023 15:40

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Tgt Ion: 43 Resp: 40313
 Ion Ratio Lower Upper
 43 100
 58 35.0 0.0 74.4

