


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110823\
Data File : VU056110.D
Acq On : 08 Nov 2023 08:20
Operator : MD/SY
Sample : BFB068
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB068

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 08 20:49:31 2023

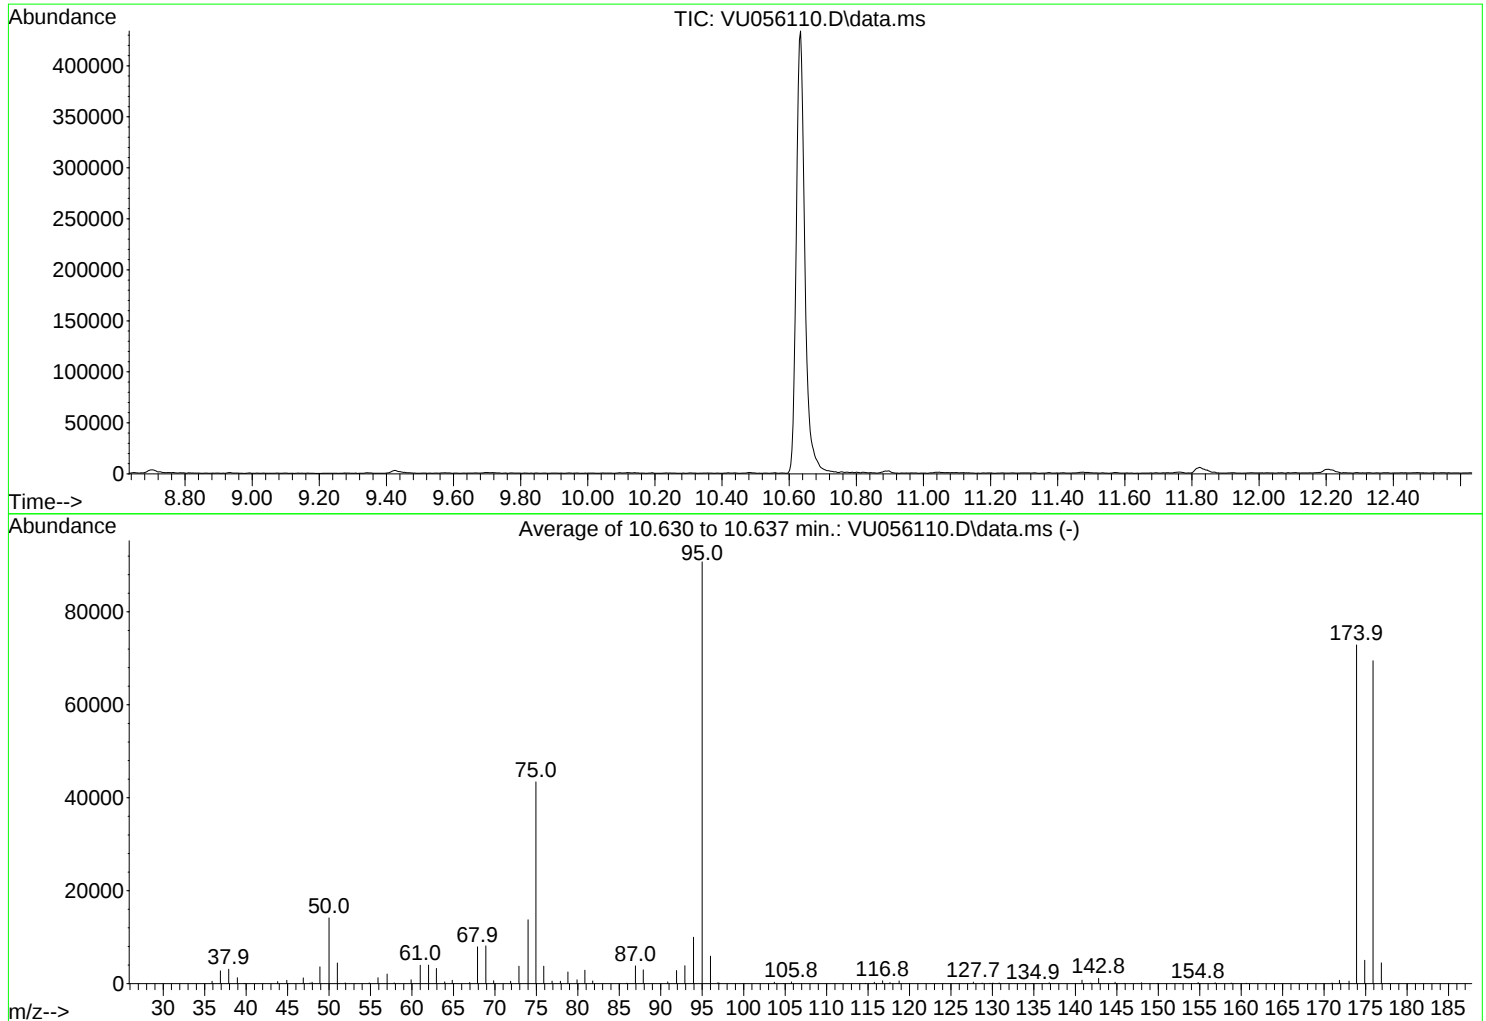

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	14154	PASS
75	95	30	80	47.8	43405	PASS
95	95	100	100	100.0	90765	PASS
96	95	5	9	6.5	5909	PASS
173	174	0.00	2	0.8	555	PASS
174	95	50	120	80.3	72888	PASS
175	174	5	9	6.9	5047	PASS
176	174	95	101	95.3	69475	PASS
177	176	5	9	6.4	4468	PASS

Scan 2892 (10.589 min): VU056110.D\data.ms
BFB068

m/z	Abundance
39.70	239.0
43.80	457.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	524.0
36.90	2967.0
37.90	3141.0
38.90	1415.0
39.80	310.0
43.90	906.0
44.90	721.0
46.90	1176.0
48.00	470.0
48.90	3594.0
50.00	14573.0
51.00	4569.0
51.90	156.0
55.00	207.0
55.90	1319.0
57.00	2005.0
57.80	102.0
59.90	927.0
61.00	4009.0
62.00	3883.0
63.00	3154.0
63.90	368.0
64.80	690.0
66.90	204.0
67.90	7763.0
68.90	8549.0
69.90	679.0
71.90	616.0
72.90	3748.0
74.00	13992.0
75.00	44224.0
75.90	3631.0
76.90	621.0
77.90	574.0
78.80	2431.0
79.90	777.0
80.90	2824.0
81.80	634.0
85.90	152.0
87.00	3649.0
87.90	3290.0
90.80	316.0
91.90	3003.0
92.90	3863.0
94.00	9992.0
95.00	91752.0
96.00	5936.0
96.90	278.0
97.10	284.0
103.70	278.0
105.80	413.0
115.70	321.0
116.80	657.0
117.80	250.0
118.80	526.0
127.70	326.0
128.70	146.0
129.70	192.0
130.80	149.0
136.90	140.0
140.70	830.0
141.90	153.0
142.80	1113.0
144.80	309.0
145.90	126.0
148.00	291.0
152.70	113.0
154.80	264.0
156.90	233.0
158.80	150.0
171.00	101.0
171.80	668.0
173.00	487.0
173.90	72744.0
174.90	5117.0
175.90	69832.0
176.90	4547.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	565.0
36.90	2763.0
37.90	3186.0
38.90	1330.0
39.80	332.0
43.80	872.0
44.90	732.0
46.90	1275.0
47.90	425.0
48.90	3737.0
50.00	14517.0
51.00	4586.0
51.90	189.0
54.80	176.0
55.90	1309.0
57.00	2108.0
57.90	203.0
59.90	879.0
61.00	4101.0
62.00	4146.0
62.90	3390.0
63.90	393.0
64.90	745.0
67.00	278.0
67.90	8282.0
68.90	8293.0
69.80	662.0
71.90	500.0
72.90	3905.0
74.00	14252.0
74.90	44496.0
75.90	3855.0
76.90	575.0
77.90	575.0
78.80	2634.0
79.90	844.0
80.80	2966.0
81.80	592.0
85.90	141.0
87.00	3941.0
87.90	3040.0
90.90	396.0
91.90	2949.0
92.90	4029.0
94.00	10274.0
95.00	93336.0
96.00	6114.0
96.90	254.0
103.70	347.0
105.80	392.0
114.70	122.0
115.80	338.0
116.80	651.0
117.60	232.0
118.70	611.0
127.70	356.0
128.70	132.0
129.70	153.0
130.00	146.0
130.70	146.0
130.90	147.0
136.80	207.0
140.80	780.0
141.90	138.0
142.80	1192.0
144.80	346.0
145.90	109.0
148.00	218.0
149.90	107.0
152.70	106.0
154.80	253.0
156.80	192.0
158.80	151.0
160.60	128.0
170.90	135.0
171.80	739.0
173.00	579.0
173.90	74832.0
174.90	5113.0
175.90	71184.0
176.90	4536.0
177.80	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	507.0
36.90	2527.0
37.90	2929.0
39.00	1066.0
39.80	298.0
43.80	893.0
44.90	680.0
46.90	1234.0
47.70	423.0
48.90	3536.0
50.00	13372.0
51.00	4181.0
52.00	174.0
54.80	144.0
55.90	1209.0
57.00	2117.0
57.90	241.0
59.90	734.0
61.00	3790.0
62.00	3918.0
62.90	3315.0
64.00	377.0
64.90	747.0
67.00	277.0
67.90	7706.0
68.90	7524.0
69.80	573.0
71.90	405.0
72.90	3572.0
74.00	12966.0
74.90	41496.0
75.90	3757.0
76.90	464.0
77.90	441.0
78.80	2503.0
79.90	820.0
80.80	2867.0
81.80	531.0
86.90	3835.0
87.90	2590.0
90.90	482.0
91.90	2523.0
92.90	3727.0
93.90	9728.0
95.00	87208.0
96.00	5678.0
96.90	201.0
103.70	361.0
104.80	122.0
105.70	359.0
114.70	119.0
115.70	310.0
116.70	515.0
117.60	212.0
118.70	595.0
127.70	317.0
128.80	127.0
130.10	231.0
130.90	101.0
134.90	135.0
136.80	238.0
140.90	686.0
141.70	103.0
142.80	1159.0
144.80	305.0
147.80	150.0
149.90	126.0
154.80	244.0
156.80	223.0
158.80	121.0
160.60	171.0
170.90	141.0
171.90	762.0
173.00	598.0
173.90	71088.0
174.90	4910.0
175.90	67408.0
176.90	4320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068