
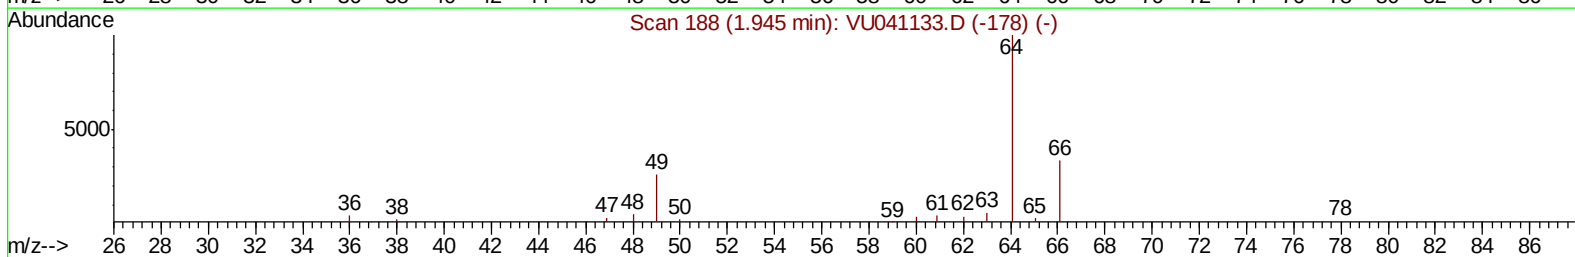
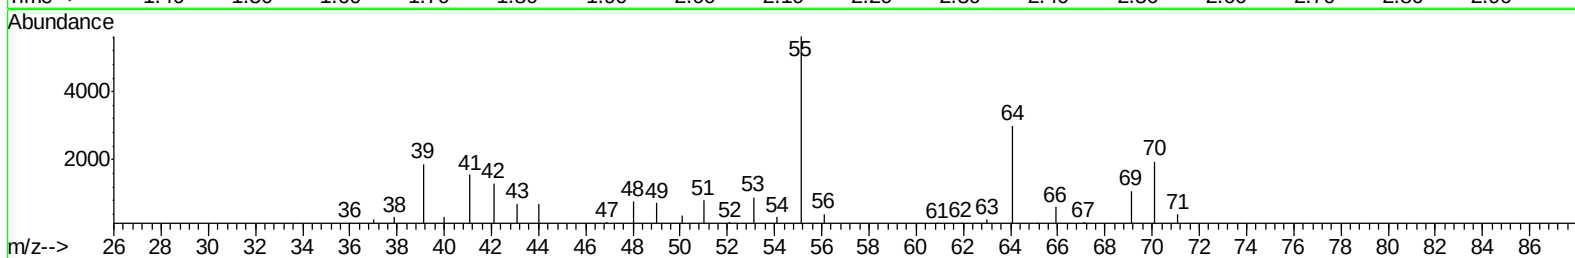


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110920\
 Data File : VU041147.D
 Acq On : 09 Nov 2020 17:41
 Operator : SY/MD
 Sample : L4646-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 10 01:13:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 10 01:04:12 2020
 Response via : Initial Calibration

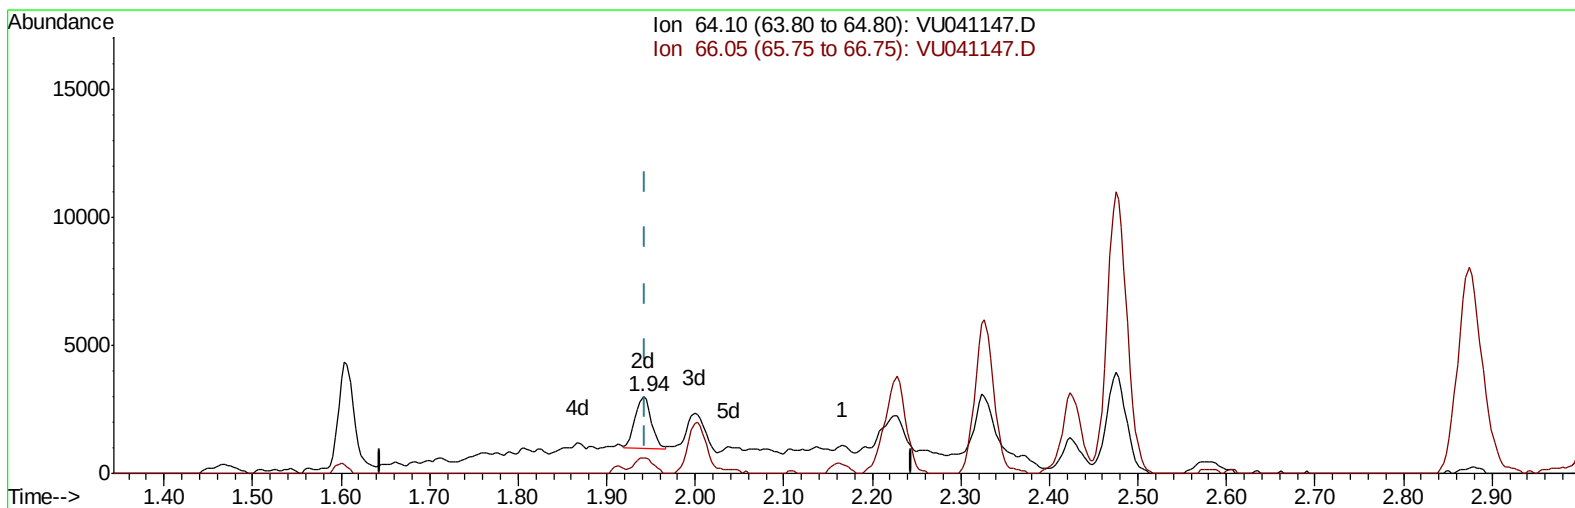

TIC: VU041147.D

(8) Chloroethane (T)

1.941min (-0.003) 0.63ug/L m

response 2579

Ion	Exp%	Act%
64.10	100	100
66.05	31.90	19.99#
0.00	0.00	0.00
0.00	0.00	0.00