


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU110920\
 Data File : VU041132.D
 Acq On : 09 Nov 2020 09:29
 Operator : SY/MD
 Sample : BFB08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 11 00:43:53 2020

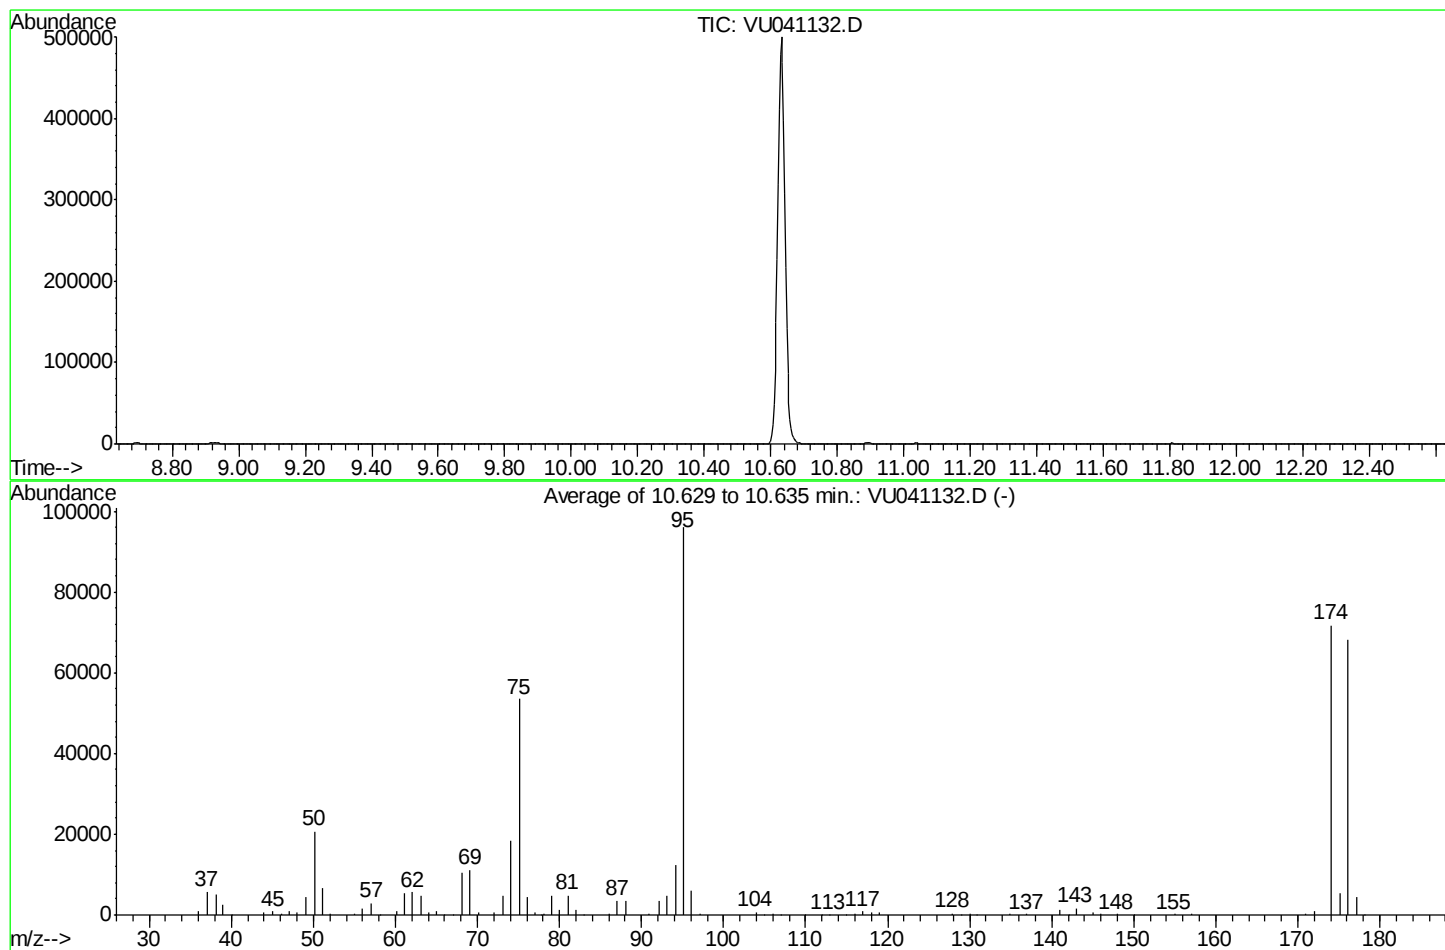

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	20744	PASS
75	95	30	80	55.8	53560	PASS
95	95	100	100	100.0	96016	PASS
96	95	5	9	6.4	6140	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.6	71672	PASS
175	174	5	9	7.4	5311	PASS
176	174	95	101	95.2	68213	PASS
177	176	5	9	6.7	4546	PASS

m/z	Abundance
36.00	898.0
37.10	5740.0
38.10	4990.0
39.00	2360.0
40.00	134.0
44.00	769.0
45.10	906.0
46.10	160.0
47.10	1084.0
48.00	688.0
49.00	4752.0
50.10	21080.0
51.10	6764.0
52.00	310.0
55.00	373.0
56.00	1657.0
57.10	2927.0
58.20	120.0
60.10	998.0
61.10	5390.0
62.10	5753.0
63.10	4950.0
64.00	865.0
65.10	1003.0
66.00	114.0
67.10	311.0
68.10	10555.0
69.10	11081.0
70.10	767.0
72.00	655.0
73.10	4787.0
74.10	18400.0
75.10	53480.0
76.10	4542.0
77.00	604.0
77.80	301.0
78.10	301.0
79.00	4759.0
80.00	1284.0
81.00	4941.0
82.00	1144.0
82.90	132.0
86.10	155.0
87.00	3644.0
88.00	3376.0
90.90	412.0
92.10	3295.0
93.10	5025.0
94.10	12307.0
95.10	94848.0
96.10	6147.0
97.10	204.0
104.00	629.0
104.90	130.0
106.00	428.0
107.00	107.0
114.80	106.0
116.00	514.0
117.00	907.0
118.00	525.0
119.00	682.0
127.90	321.0
128.90	123.0
130.00	353.0
130.90	117.0
135.00	222.0
137.00	218.0
141.00	1256.0
142.00	188.0
143.00	1707.0
145.10	657.0
145.90	180.0
148.00	199.0
155.00	192.0
157.00	196.0
171.00	311.0
172.10	1019.0
174.10	69712.0
175.10	4990.0
176.10	66192.0
177.10	4399.0
178.10	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	1061.0
37.10	6028.0
38.10	5280.0
39.00	2538.0
40.00	123.0
44.00	831.0
45.10	941.0
46.10	183.0
47.10	1010.0
48.00	757.0
49.00	4587.0
50.10	21568.0
51.10	6882.0
52.00	302.0
55.00	379.0
56.00	1719.0
57.10	3026.0
60.10	1075.0
61.10	5518.0
62.10	5838.0
63.10	4934.0
64.00	785.0
65.10	898.0
65.90	117.0
68.10	10875.0
69.10	11566.0
70.10	792.0
72.10	617.0
73.10	4968.0
74.10	18952.0
75.10	55704.0
76.10	4706.0
77.10	586.0
78.10	303.0
79.00	4885.0
80.00	1314.0
81.00	5024.0
82.00	1215.0
82.90	109.0
86.10	218.0
87.10	3663.0
88.00	3531.0
90.90	420.0
92.10	3493.0
93.10	5097.0
94.10	12819.0
95.10	99224.0
96.10	6362.0
97.10	193.0
104.00	672.0
105.00	148.0
106.00	477.0
107.00	100.0
109.90	103.0
112.90	119.0
114.90	113.0
116.00	506.0
117.00	971.0
118.00	535.0
119.00	775.0
127.90	362.0
129.00	180.0
130.00	344.0
130.80	151.0
134.90	229.0
137.00	239.0
141.00	1279.0
142.00	172.0
143.00	1721.0
145.10	584.0
145.90	190.0
148.00	200.0
155.00	225.0
157.00	186.0
171.00	319.0
172.10	1101.0
174.10	74480.0
175.10	5538.0
176.10	70696.0
177.10	4718.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	1093.0
37.00	5587.0
38.10	4962.0
39.00	2298.0
40.00	125.0
44.00	800.0
45.00	860.0
46.10	179.0
47.10	907.0
48.00	700.0
49.10	4075.0
50.10	19584.0
51.10	6202.0
52.00	231.0
55.00	313.0
56.00	1584.0
57.10	2972.0
60.10	998.0
61.10	5135.0
62.10	5296.0
63.10	4402.0
64.00	656.0
65.00	753.0
65.90	113.0
68.10	10187.0
69.10	10758.0
70.10	674.0
72.10	578.0
73.10	4745.0
74.10	17784.0
75.10	51496.0
76.10	4392.0
77.00	494.0
78.00	315.0
79.00	4470.0
80.00	1301.0
81.00	4645.0
82.00	1146.0
86.10	202.0
87.10	3456.0
88.10	3478.0
90.90	399.0
92.10	3249.0
93.10	4546.0
94.10	11952.0
95.10	93976.0
96.10	5912.0
97.10	158.0
103.90	671.0
105.00	139.0
106.00	484.0
107.00	108.0
111.90	107.0
112.80	167.0
115.00	113.0
116.00	433.0
117.00	943.0
118.00	479.0
119.00	718.0
127.90	336.0
129.00	204.0
130.00	289.0
130.80	149.0
134.90	182.0
137.00	228.0
141.00	1156.0
142.00	134.0
143.00	1492.0
145.10	460.0
146.00	190.0
148.00	187.0
150.00	103.0
155.00	219.0
157.00	193.0
171.00	270.0
172.10	993.0
174.10	70824.0
175.10	5406.0
176.10	67752.0
177.10	4521.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
44.00	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08