
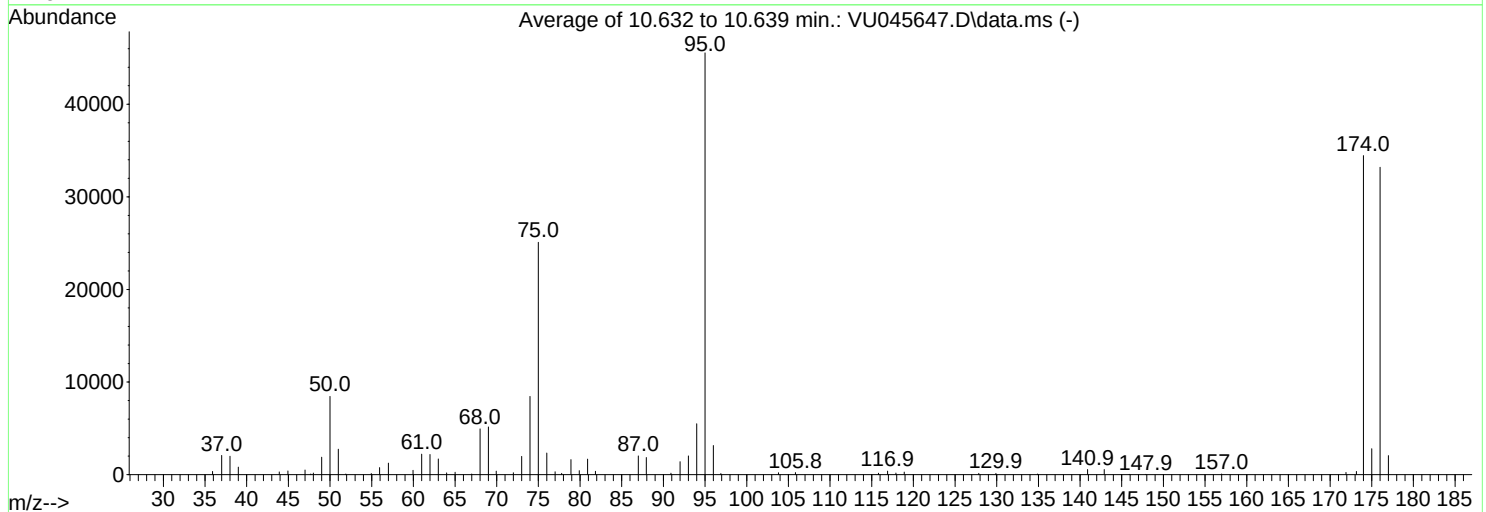


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110921\
 Data File : VU045647.D
 Acq On : 09 Nov 2021 09:47
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260
 Last Update : Fri Nov 05 13:35:16 2021

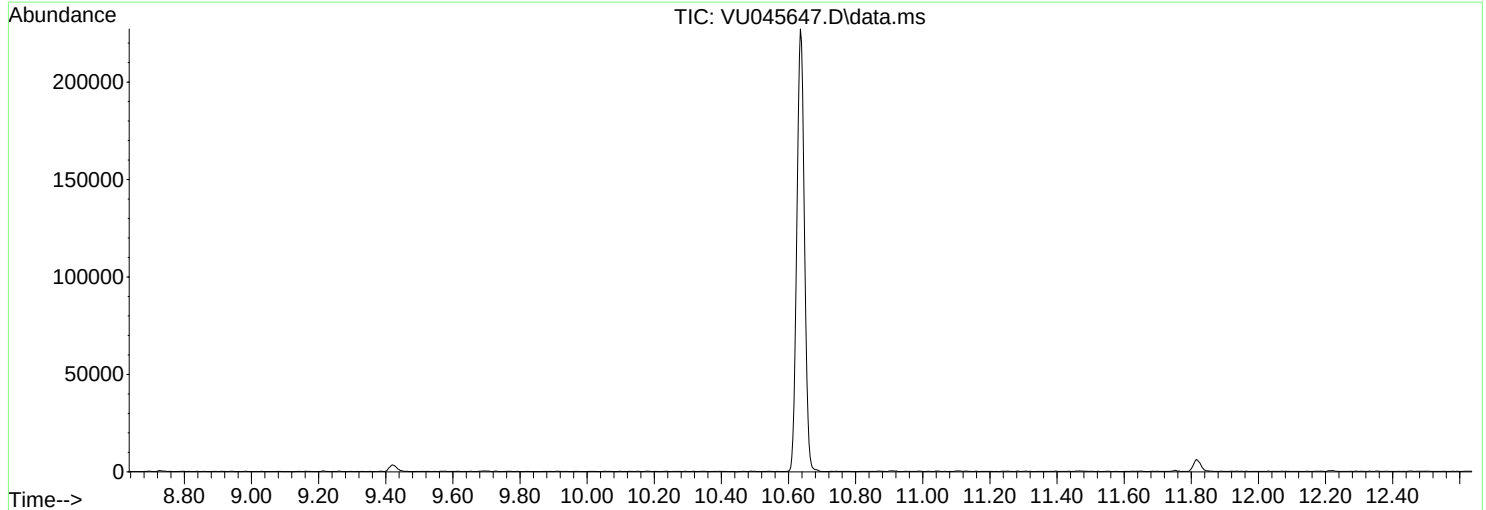

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	8450	PASS
75	95	30	60	55.1	25093	PASS
95	95	100	100	100.0	45552	PASS
96	95	5	9	6.9	3149	PASS
173	174	0.00	2	1.0	340	PASS
174	95	50	100	75.6	34451	PASS
175	174	5	9	8.2	2808	PASS
176	174	95	101	96.4	33195	PASS
177	176	5	9	6.2	2059	PASS