
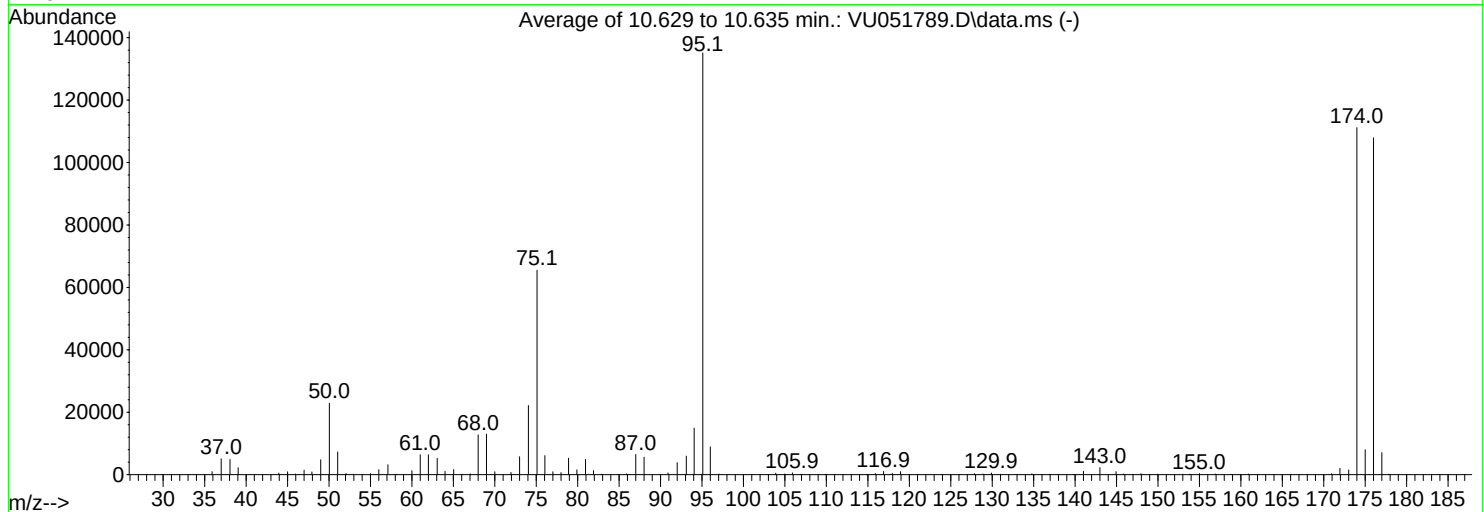


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110922\
 Data File : VU051789.D
 Acq On : 09 Nov 2022 08:58
 Operator : JC/MD
 Sample : BFB166
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB166

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 10 01:04:23 2022

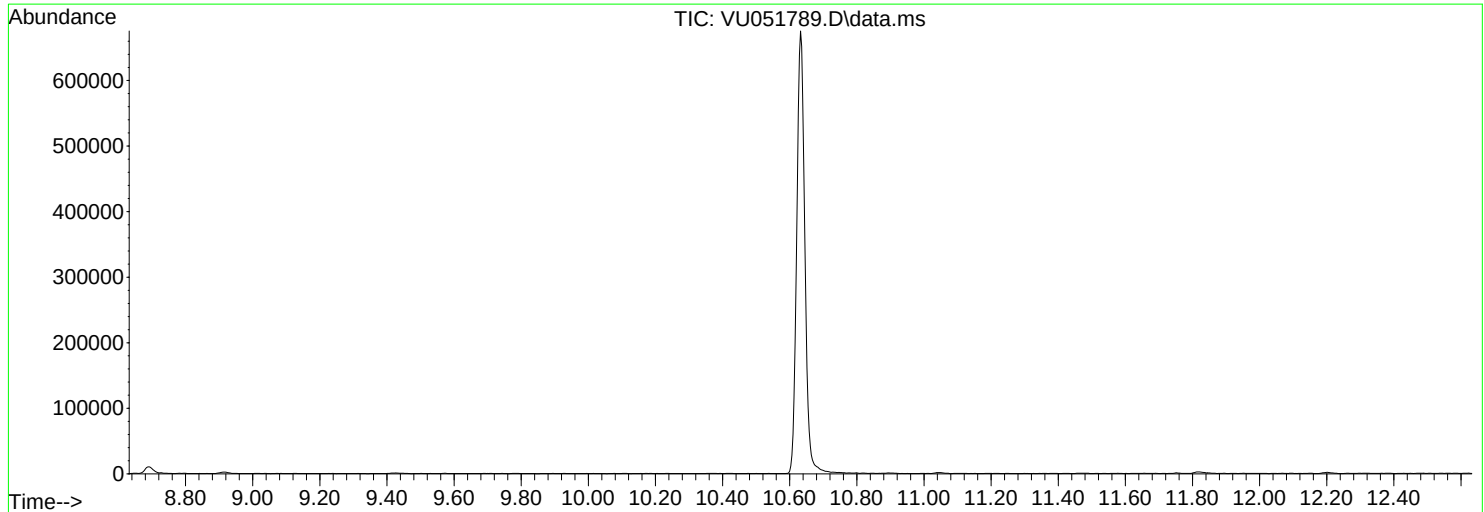

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	22888	PASS
75	95	30	80	48.5	65525	PASS
95	95	100	100	100.0	135147	PASS
96	95	5	9	6.6	8918	PASS
173	174	0.00	2	1.4	1515	PASS
174	95	50	120	82.3	111195	PASS
175	174	5	9	7.2	8009	PASS
176	174	95	101	97.1	107928	PASS
177	176	5	9	6.6	7079	PASS

Scan 2876 (10.587 min): VU051789.D\data.ms
BFB166

m/z	Abundance
40.00	128.0
43.90	477.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	967.0
37.00	5102.0
38.00	4693.0
39.10	2341.0
40.10	290.0
44.00	982.0
45.00	954.0
46.00	194.0
47.00	1400.0
47.90	688.0
49.00	4682.0
50.00	22640.0
51.00	7019.0
52.00	375.0
53.00	152.0
55.00	293.0
56.00	1628.0
57.10	3015.0
58.20	119.0
60.00	1290.0
61.00	6325.0
62.00	6342.0
63.00	5213.0
64.00	1028.0
65.10	1585.0
66.00	203.0
67.10	239.0
68.00	12292.0
69.00	12698.0
70.00	908.0
72.00	732.0
73.00	5785.0
74.00	21968.0
75.10	64560.0
76.00	6092.0
77.00	773.0
78.00	691.0
78.90	5302.0
79.90	1420.0
80.90	4677.0
81.90	1262.0
82.90	130.0
85.90	258.0
87.00	6198.0
88.00	5396.0
90.90	526.0
92.00	3966.0
93.10	5595.0
94.00	14821.0
95.10	133568.0
96.00	9060.0
97.10	224.0
103.90	466.0
105.00	231.0
105.90	492.0
110.90	105.0
114.90	117.0
115.90	304.0
116.90	1016.0
118.00	491.0
118.90	1022.0
127.90	337.0
128.90	198.0
129.90	556.0
131.00	142.0
134.80	306.0
136.90	129.0
141.00	1004.0
142.00	134.0
143.00	2283.0
144.00	107.0
145.00	1007.0
145.90	185.0
146.90	116.0
147.90	296.0
150.00	109.0
153.00	170.0
153.80	117.0
155.00	290.0
156.90	226.0
158.90	101.0
160.90	176.0
170.90	320.0
171.90	1919.0
173.00	1415.0
174.00	106664.0
175.00	7692.0
176.00	102736.0
177.00	7008.0
177.80	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	1073.0
37.00	5165.0
38.10	5047.0
39.10	2277.0
40.10	247.0
44.00	996.0
45.00	960.0
46.00	220.0
47.00	1443.0
47.90	887.0
49.00	4866.0
50.10	23576.0
51.10	7498.0
52.00	342.0
52.90	198.0
55.00	336.0
56.00	1592.0
57.10	3272.0
58.20	145.0
60.00	1324.0
61.00	6588.0
62.00	6548.0
63.00	5377.0
64.00	1056.0
65.00	1677.0
66.10	169.0
67.10	266.0
68.00	13162.0
69.00	13388.0
70.00	934.0
71.90	757.0
73.00	5929.0
74.10	22912.0
75.10	67608.0
76.10	6321.0
77.00	937.0
78.00	718.0
78.90	5549.0
79.90	1595.0
81.00	5086.0
81.90	1342.0
82.90	151.0
85.90	293.0
87.00	6750.0
88.00	5757.0
90.90	614.0
92.00	3957.0
93.10	6093.0
94.00	15507.0
95.10	139200.0
96.00	9164.0
97.10	227.0
103.90	467.0
104.90	223.0
105.90	578.0
106.90	111.0
109.90	105.0
114.90	144.0
115.90	376.0
116.90	1043.0
117.90	473.0
118.90	1049.0
126.00	105.0
127.80	397.0
128.90	233.0
129.90	532.0
131.00	181.0
134.80	309.0
136.90	136.0
141.00	1105.0
141.90	114.0
143.00	2348.0
145.00	1048.0
145.90	195.0
146.90	136.0
148.00	315.0
150.00	151.0
153.00	175.0
153.80	158.0
155.00	368.0
156.90	221.0
158.90	100.0
160.90	196.0
170.90	282.0
172.00	2092.0
173.00	1536.0
174.00	114160.0
175.00	8152.0
176.00	111512.0
177.00	7360.0
177.80	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	968.0
37.00	4979.0
38.10	4804.0
39.00	2036.0
40.10	198.0
44.00	979.0
45.00	865.0
45.90	211.0
47.00	1409.0
48.00	1023.0
49.00	4837.0
50.10	22448.0
51.10	7272.0
52.10	348.0
52.90	196.0
55.00	365.0
56.00	1541.0
57.10	3313.0
58.20	141.0
60.00	1307.0
61.00	6235.0
62.00	6176.0
63.10	5058.0
64.00	1090.0
65.00	1660.0
66.10	135.0
67.00	300.0
68.00	12897.0
69.00	12886.0
70.00	886.0
72.00	688.0
73.00	5552.0
74.10	21568.0
75.10	64408.0
76.10	5872.0
77.00	1002.0
78.00	635.0
78.90	5060.0
79.90	1645.0
80.90	4931.0
81.90	1254.0
82.90	130.0
85.90	283.0
87.00	6381.0
88.00	5589.0
90.90	601.0
92.00	3621.0
93.10	6142.0
94.10	14520.0
95.10	132672.0
96.00	8529.0
97.00	239.0
103.90	480.0
104.90	204.0
105.90	581.0
106.80	116.0
114.90	157.0
115.90	422.0
116.90	996.0
117.90	437.0
119.00	869.0
127.90	405.0
128.90	209.0
129.90	517.0
131.00	181.0
134.80	230.0
136.90	136.0
139.80	102.0
141.00	1118.0
141.90	125.0
143.00	2178.0
144.90	960.0
145.80	201.0
146.90	135.0
147.90	359.0
149.90	151.0
153.00	135.0
153.80	138.0
155.00	374.0
157.00	220.0
158.90	120.0
160.90	187.0
171.00	293.0
172.00	2016.0
173.00	1595.0
174.00	112760.0
175.00	8184.0
176.00	109536.0
177.00	6868.0
177.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166