

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
 Data File : VU056136.D
 Acq On : 09 Nov 2023 13:34
 Operator : MD/SY
 Sample : 05297-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B24

Quant Time: Nov 09 21:35:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 09 21:34:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	406932	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	407567	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	178015	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	113587	4.497	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.000%
7) Chloroethane-d5	1.908	69	92608	5.403	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.000%
11) 1,1-Dichloroethene-d2	2.563	65	51594	4.636	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.800%
20) 2-Butanone-d5	4.618	46	240601	58.064	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.120%
24) Chloroform-d	5.055	84	234076	4.868	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.698	65	110870	5.237	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	5.721	84	466172	4.762	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	6.686	67	143991	4.997	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%
41) Toluene-d8	7.894	98	396422	4.419	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.400%
43) trans-1,3-Dichloroprop...	8.177	79	49856	4.527	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.631	63	188536	52.225	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.460%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	106131	5.161	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	142363	5.186	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds						
13) Acetone	2.631	43	38594	12.629	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
Data File : VU056136.D
Acq On : 09 Nov 2023 13:34
Operator : MD/SY
Sample : 05297-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B24


Quant Time: Nov 09 21:35:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 09 21:34:15 2023
Response via : Initial Calibration

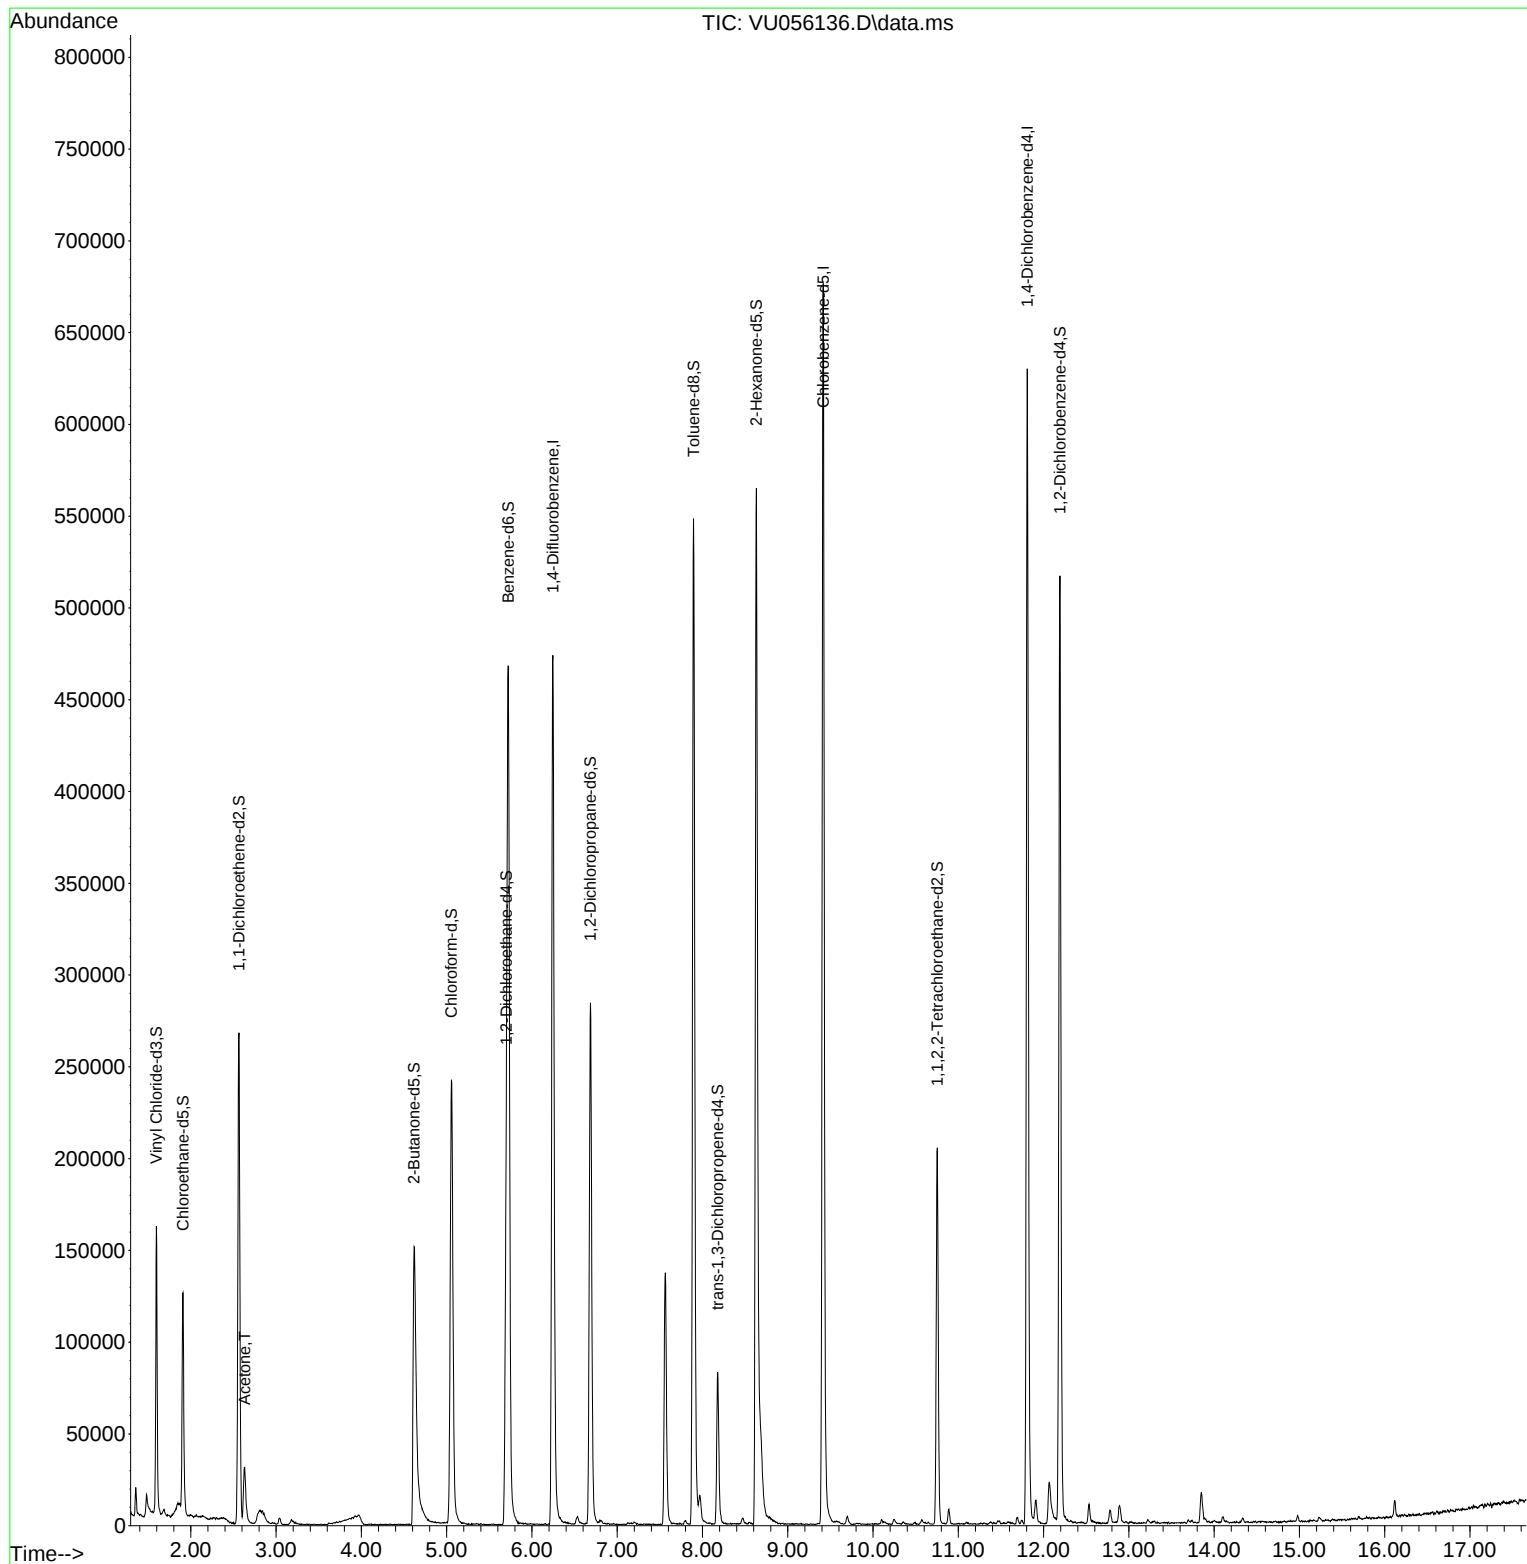

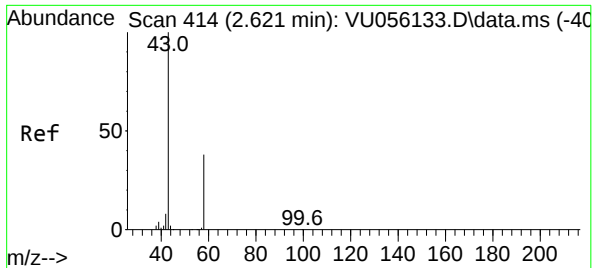

#13
Acetone
Concen: 12.629 ug/L
RT: 2.631 min Scan# 41
Delta R.T. 0.010 min
Lab File: VU056136.D
Acq: 09 Nov 2023 13:34

Instrument :
MSVOA_U
ClientSampleId :
C0B24

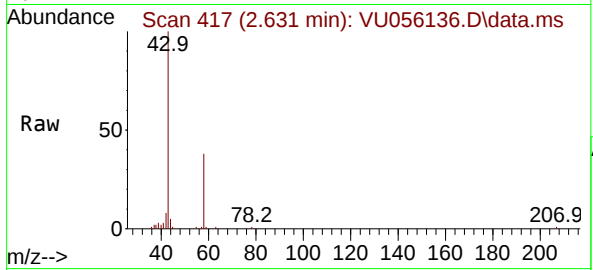

Tgt Ion: 43 Resp: 38594
Ion Ratio Lower Upper
43 100
58 39.0 0.0 74.4

