

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
 Data File : VU056153.D
 Acq On : 09 Nov 2023 20:29
 Operator : MD/SY
 Sample : 05339-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDH7

Quant Time: Nov 09 21:39:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 09 21:34:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	383915	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	382311	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	175707	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	107965	4.531	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.600%	
7) Chloroethane-d5	1.908	69	85216	5.270	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.400%	
11) 1,1-Dichloroethene-d2	2.563	65	48539	4.623	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	92.400%	
20) 2-Butanone-d5	4.621	46	286508	73.287	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	146.580%#	
24) Chloroform-d	5.055	84	233111	5.139	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	5.695	65	111086	5.562	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	111.200%	
32) Benzene-d6	5.721	84	475456	5.178	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.600%	
36) 1,2-Dichloropropane-d6	6.685	67	146190	5.409	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.200%	
41) Toluene-d8	7.894	98	401016	4.766	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
43) trans-1,3-Dichloroprop...	8.177	79	52080	5.041	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	100.800%	
46) 2-Hexanone-d5	8.627	63	228616	67.511	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	135.020%#	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	112461	5.830	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	116.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152	150072	5.538	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.800%	
Target Compounds						Qvalue
13) Acetone	2.634	43	20451	7.093	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
Data File : VU056153.D
Acq On : 09 Nov 2023 20:29
Operator : MD/SY
Sample : 05339-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDH7

Quant Time: Nov 09 21:39:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 09 21:34:15 2023
Response via : Initial Calibration

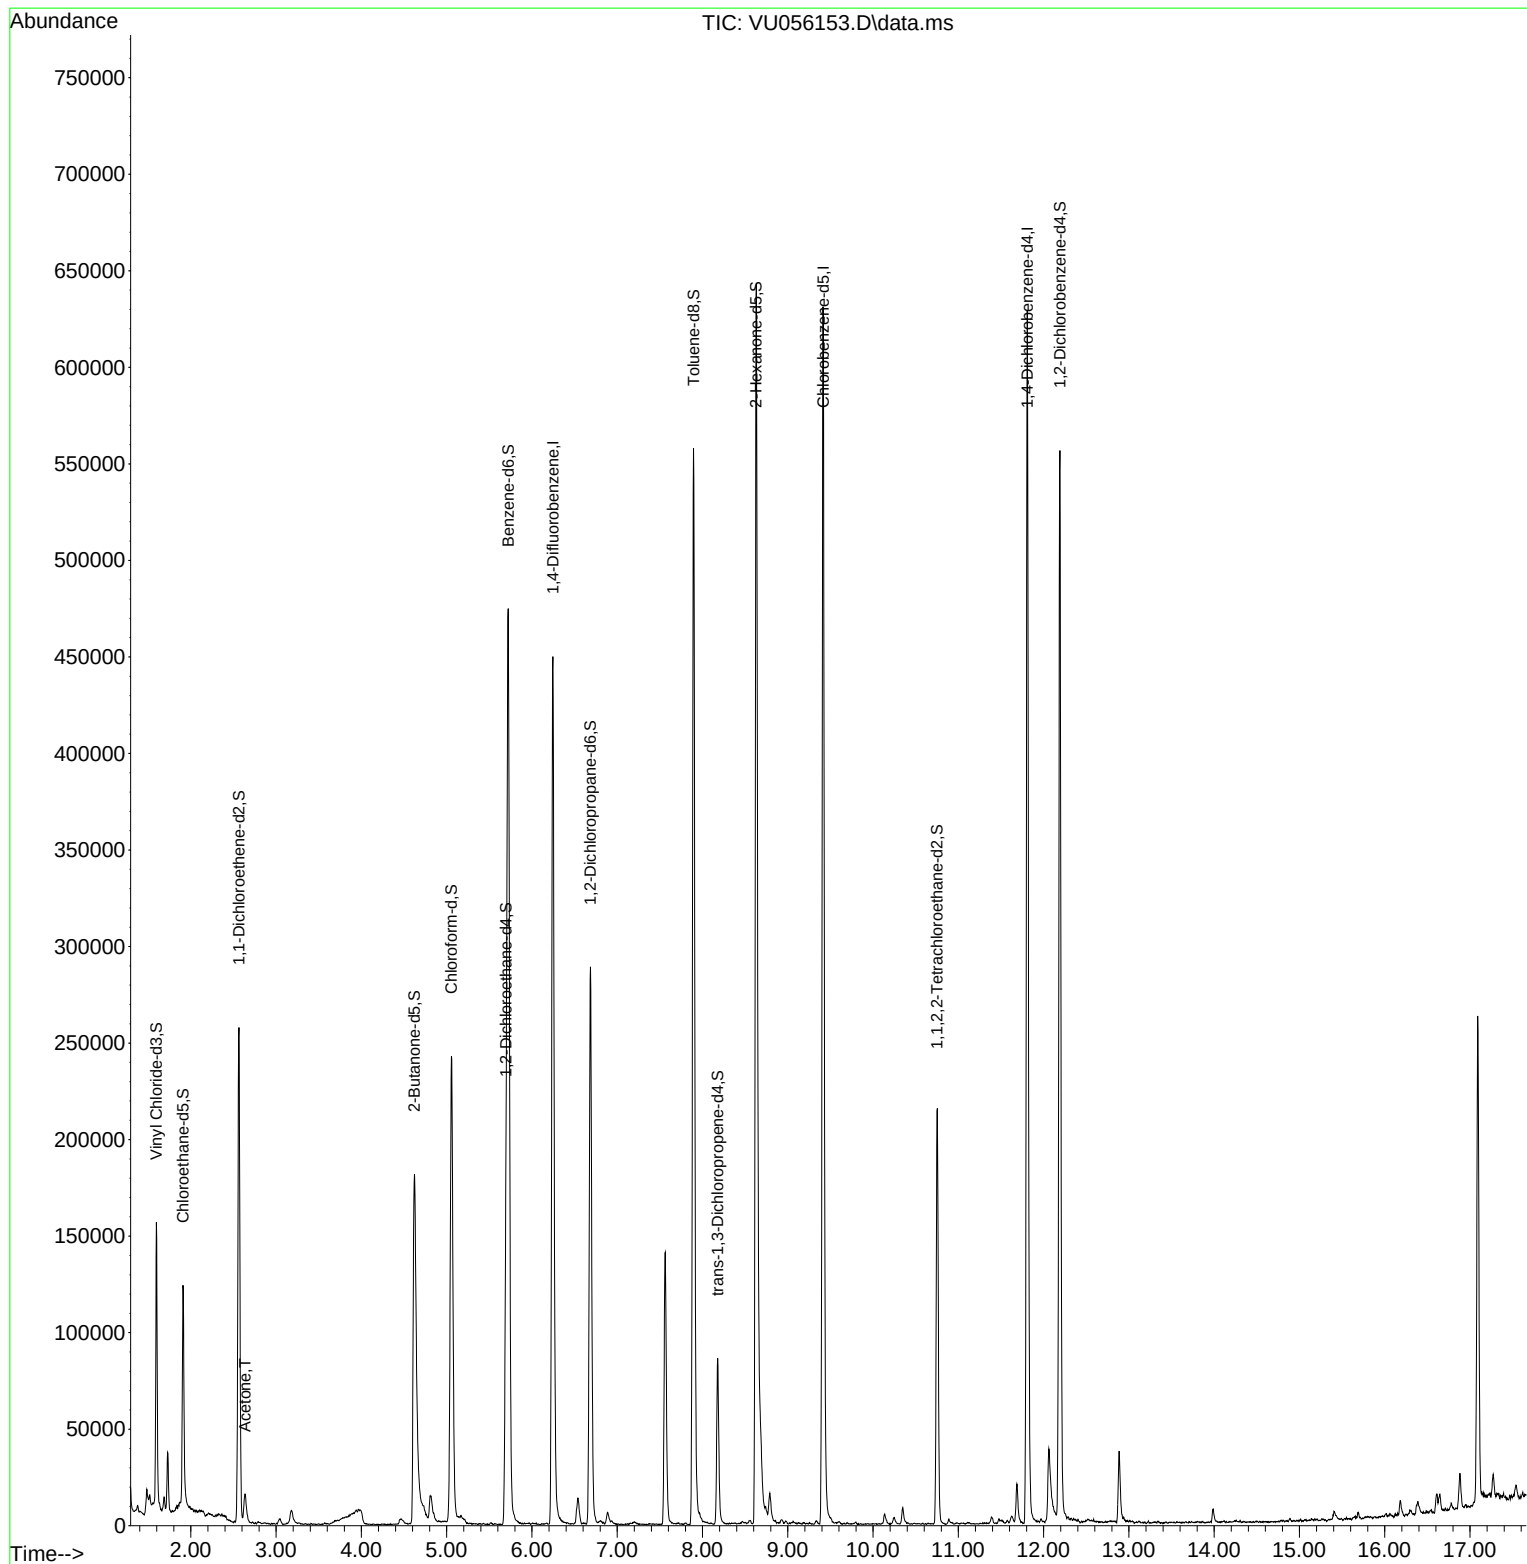

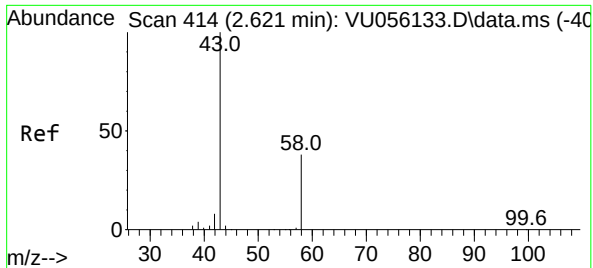

#13
 Acetone
 Concen: 7.093 ug/L
 RT: 2.634 min Scan# 41
 Delta R.T. 0.013 min
 Lab File: VU056153.D
 Acq: 09 Nov 2023 20:29

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDH7

Tgt Ion: 43 Resp: 20451
 Ion Ratio Lower Upper
 43 100
 58 37.3 0.0 74.4

