

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
 Data File : VU056154.D
 Acq On : 09 Nov 2023 20:53
 Operator : MD/SY
 Sample : 05339-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDH8

Quant Time: Nov 09 21:39:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 09 21:34:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	390686	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	391044	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	178490	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	105371	4.345	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.000%
7) Chloroethane-d5	1.911	69	87330	5.307	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%
11) 1,1-Dichloroethene-d2	2.563	65	47818	4.476	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.600%
20) 2-Butanone-d5	4.627	46	280296	70.456	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	140.920%#
24) Chloroform-d	5.055	84	230309	4.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	5.698	65	112207	5.520	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.721	84	463889	4.939	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
36) 1,2-Dichloropropane-d6	6.685	67	141588	5.121	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.894	98	394167	4.580	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	8.177	79	51474	4.871	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.400%
46) 2-Hexanone-d5	8.630	63	228449	65.955	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	131.920%#
56) 1,1,2,2-Tetrachloroeth...	10.753	84	112199	5.686	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	148629	5.400	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.000%
Target Compounds					Qvalue	
13) Acetone	2.640	43	54255	18.492	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
Data File : VU056154.D
Acq On : 09 Nov 2023 20:53
Operator : MD/SY
Sample : 05339-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDH8

Quant Time: Nov 09 21:39:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 09 21:34:15 2023
Response via : Initial Calibration

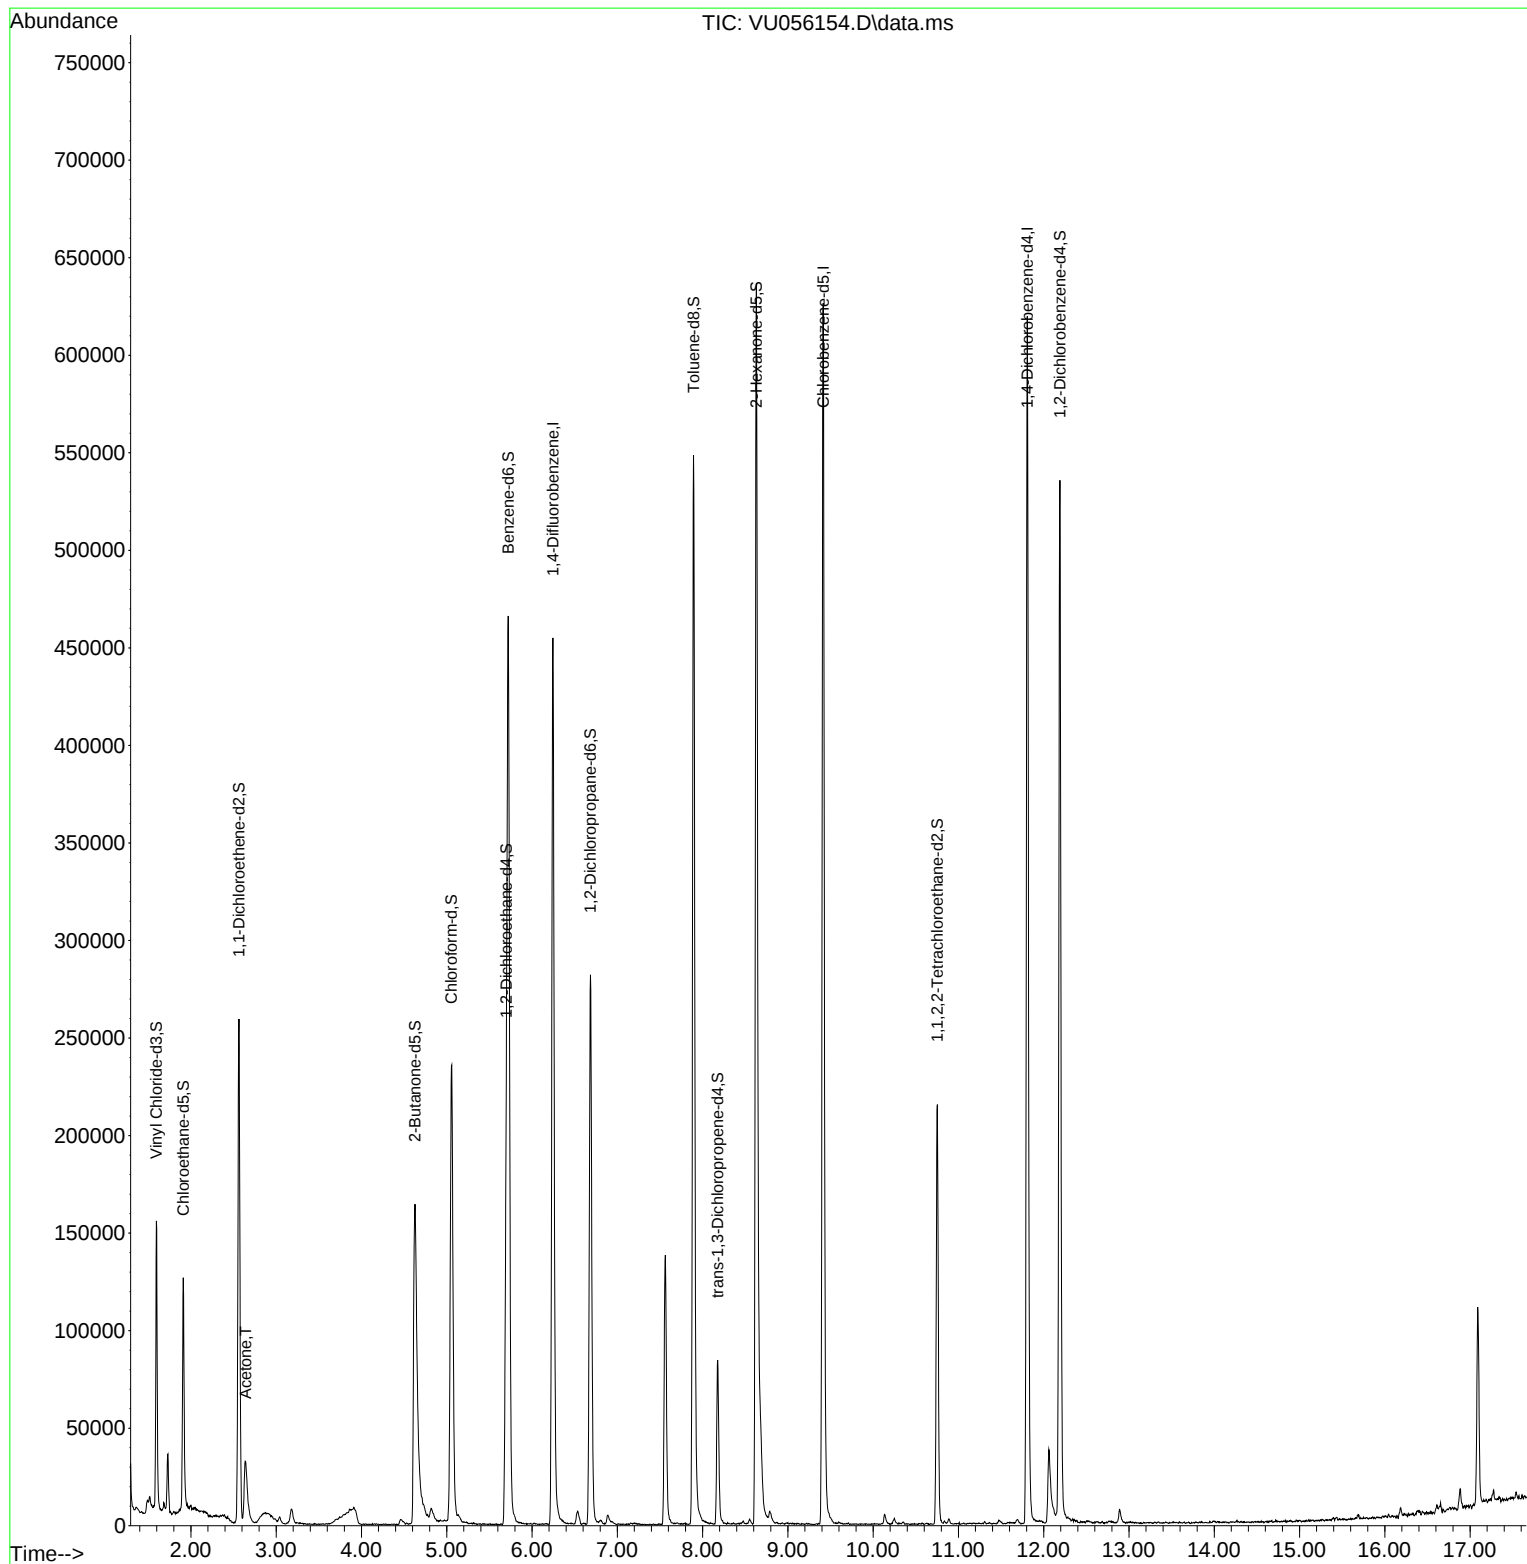

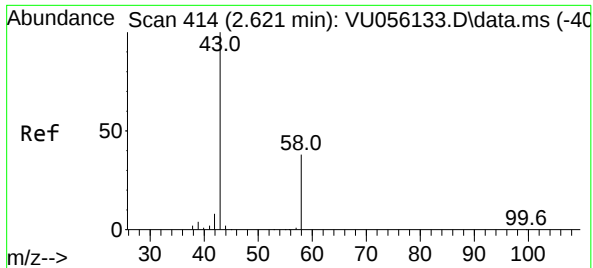

#13
 Acetone
 Concen: 18.492 ug/L
 RT: 2.640 min Scan# 41
 Delta R.T. 0.019 min
 Lab File: VU056154.D
 Acq: 09 Nov 2023 20:53

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDH8

Tgt Ion: 43 Resp: 54255
 Ion Ratio Lower Upper
 43 100
 58 38.5 0.0 74.4

