

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
 Data File : VU056155.D
 Acq On : 09 Nov 2023 21:18
 Operator : MD/SY
 Sample : 05339-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDH9

Quant Time: Nov 09 23:44:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 09 21:34:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	367948	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	374081	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	166540	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	101231	4.432	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.600%	
7) Chloroethane-d5	1.911	69	81564	5.263	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.200%	
11) 1,1-Dichloroethene-d2	2.563	65	46857	4.657	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.200%	
20) 2-Butanone-d5	4.624	46	266760	71.197	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	142.400%#	
24) Chloroform-d	5.055	84	228181	5.249	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.000%	
26) 1,2-Dichloroethane-d4	5.695	65	109156	5.702	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	114.000%	
32) Benzene-d6	5.721	84	449883	5.007	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
36) 1,2-Dichloropropane-d6	6.685	67	140090	5.297	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.000%	
41) Toluene-d8	7.894	98	384393	4.669	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.400%	
43) trans-1,3-Dichloroprop...	8.177	79	50233	4.969	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.400%	
46) 2-Hexanone-d5	8.631	63	217882	65.757	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	131.520%#	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	108543	5.750	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	115.000%	
66) 1,2-Dichlorobenzene-d4	12.190	152	144875	5.641	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.800%	
Target Compounds					Qvalue	
13) Acetone	2.634	43	24860	8.997	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
Data File : VU056155.D
Acq On : 09 Nov 2023 21:18
Operator : MD/SY
Sample : 05339-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDH9

Quant Time: Nov 09 23:44:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 09 21:34:15 2023
Response via : Initial Calibration

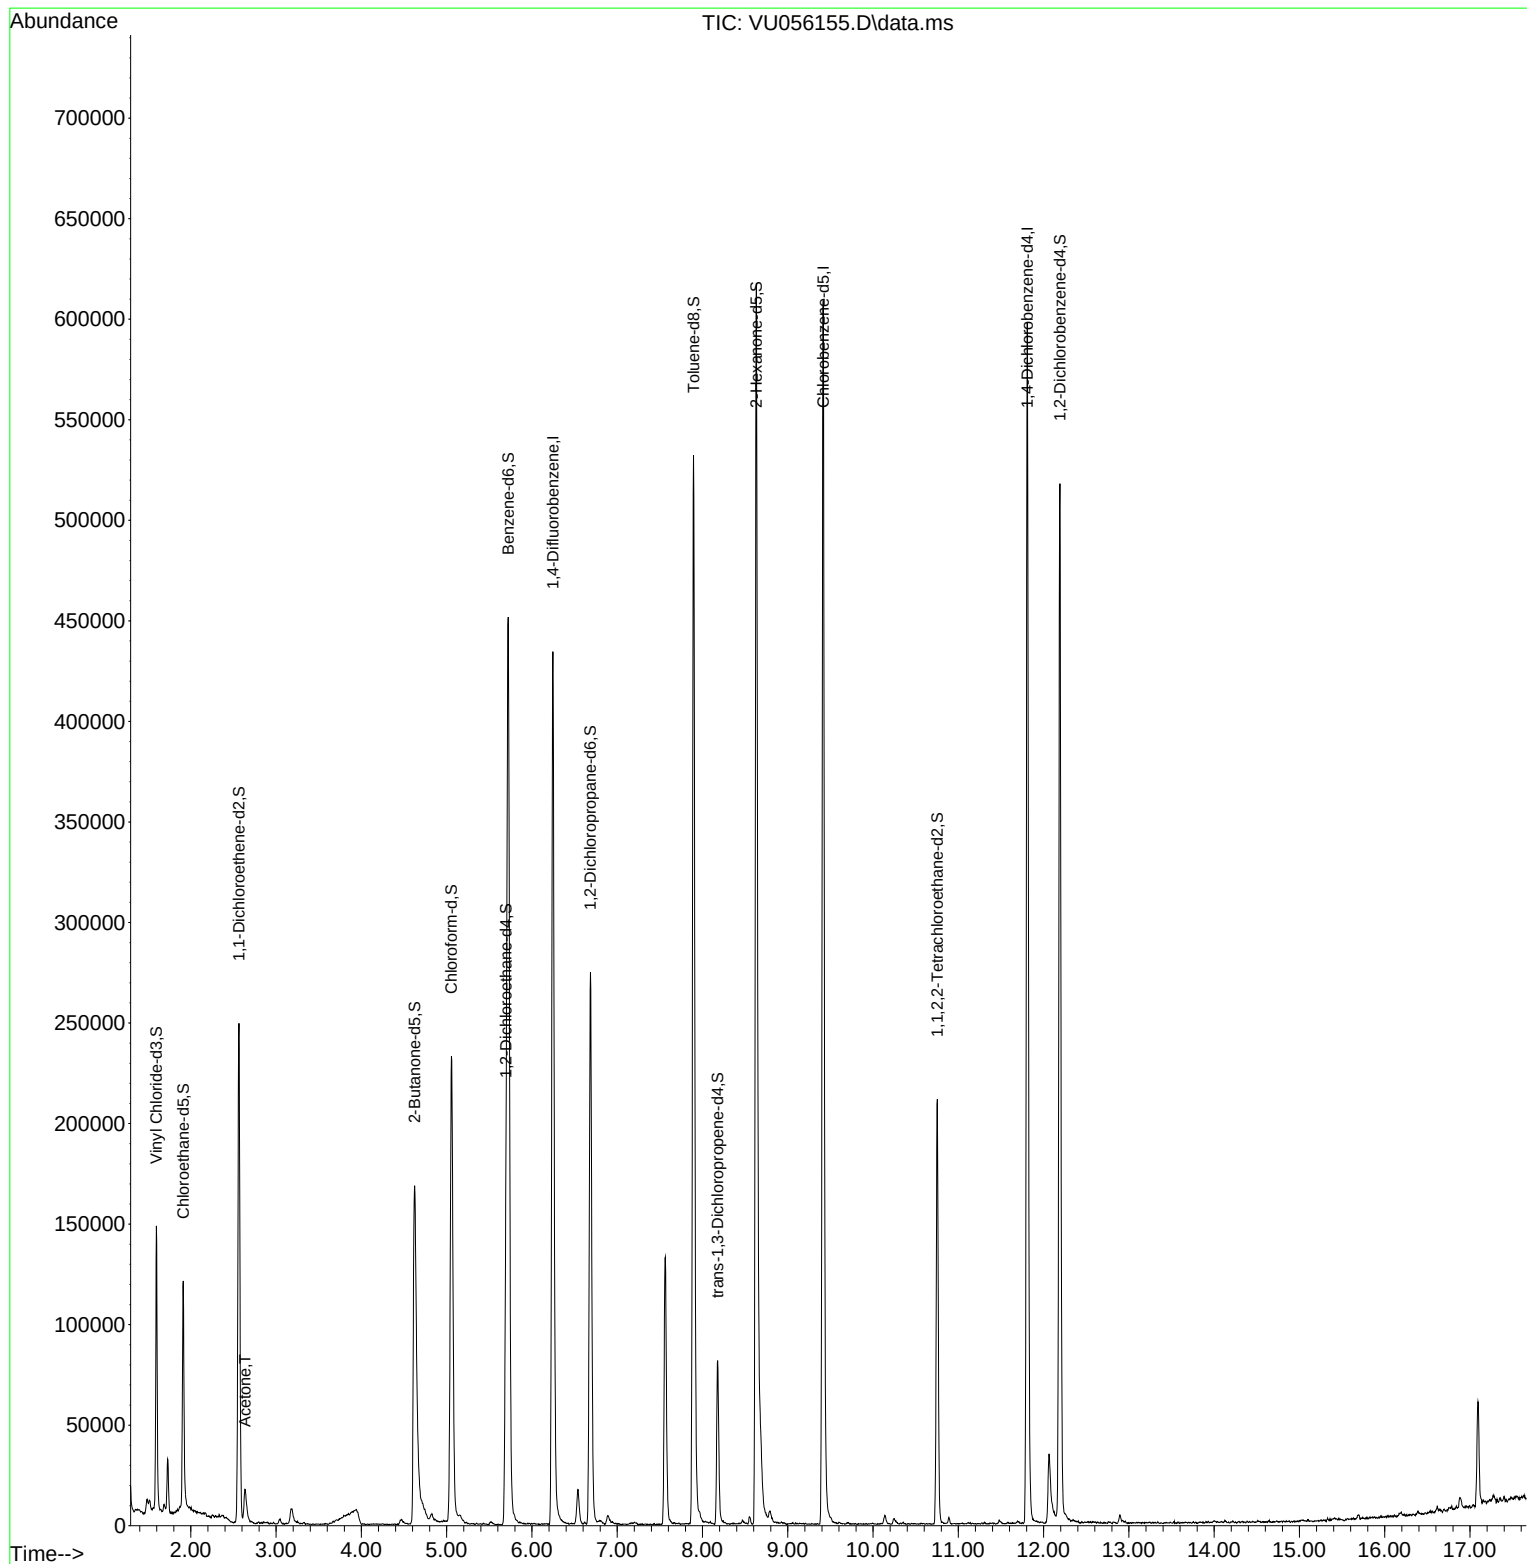

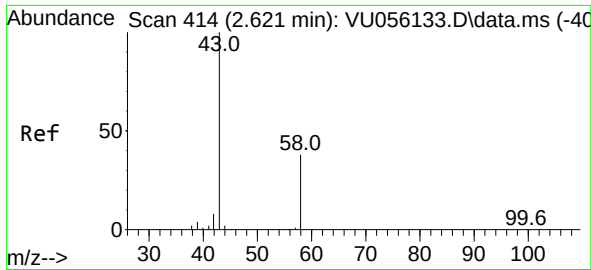

#13

Acetone

Concen: 8.997 ug/L

RT: 2.634 min Scan# 41

Delta R.T. 0.013 min

Lab File: VU056155.D


Acq: 09 Nov 2023 21:18

Instrument :

MSVOA_U

ClientSampleId :

GCDH9

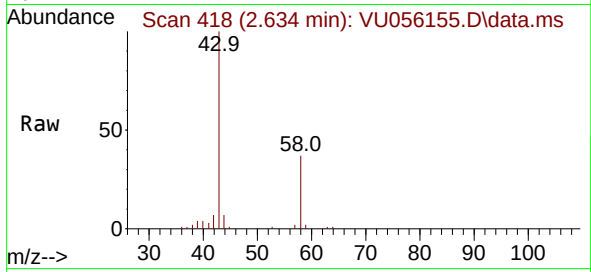

Tgt Ion: 43 Resp: 24860

Ion Ratio Lower Upper

43 100

58 37.8 0.0 74.4

