


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110923\
Data File : VU056132.D
Acq On : 09 Nov 2023 10:04
Operator : MD/SY
Sample : BFB069
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB069

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 09 21:34:15 2023

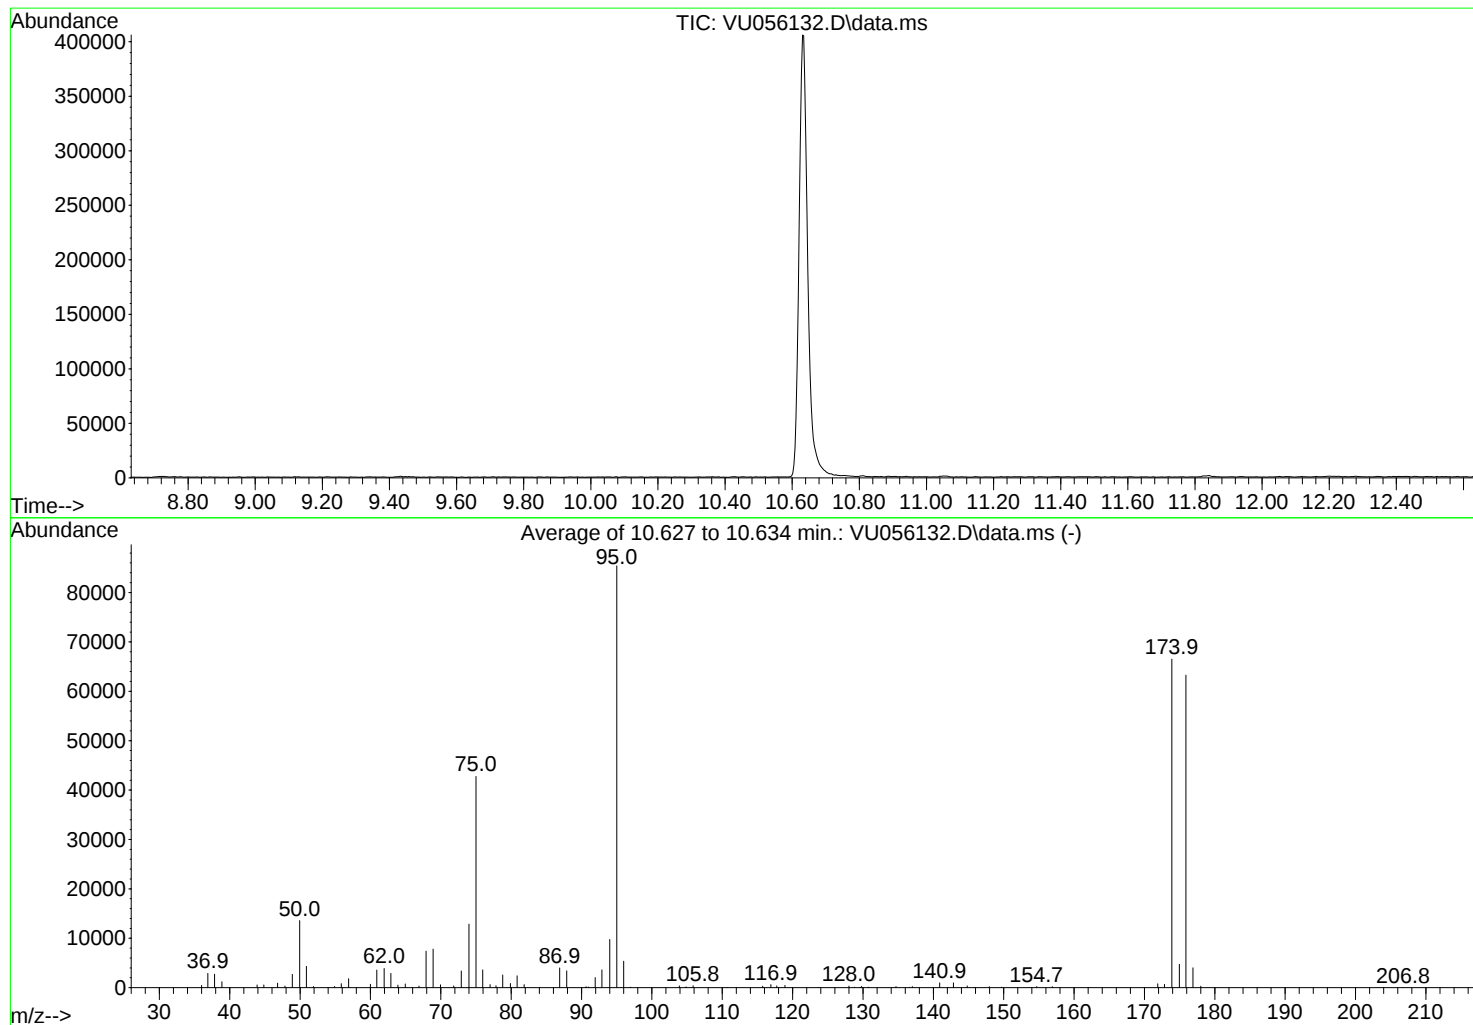

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	13575	PASS
75	95	30	80	50.1	42779	PASS
95	95	100	100	100.0	85405	PASS
96	95	5	9	6.3	5339	PASS
173	174	0.00	2	1.0	649	PASS
174	95	50	120	77.9	66525	PASS
175	174	5	9	7.1	4719	PASS
176	174	95	101	95.1	63275	PASS
177	176	5	9	6.4	4030	PASS

m/z	Abundance
39.90	339.0
43.90	447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
36.00	441.0
36.90	2732.0
37.90	2676.0
38.90	1132.0
40.00	247.0
43.90	1008.0
44.80	585.0
46.80	899.0
47.90	357.0
48.90	2710.0
50.00	12817.0
50.90	4214.0
51.90	264.0
54.90	259.0
55.90	783.0
56.90	1700.0
60.00	739.0
60.90	3530.0
62.00	3807.0
62.90	2813.0
63.90	479.0
65.00	634.0
66.90	303.0
67.90	6914.0
68.90	7479.0
69.90	526.0
71.80	273.0
72.90	3274.0
74.00	12345.0
75.00	40968.0
76.00	3463.0
77.00	617.0
77.90	367.0
78.80	2538.0
79.90	840.0
80.90	2287.0
81.80	589.0
86.90	3666.0
87.90	3144.0
90.70	200.0
91.90	1924.0
92.90	3473.0
94.00	9310.0
95.00	81040.0
96.00	5322.0
97.10	116.0
103.90	339.0
104.80	127.0
105.90	302.0
115.80	343.0
116.90	646.0
117.70	338.0
118.90	411.0
128.00	319.0
129.60	229.0
130.70	101.0
134.70	174.0
137.00	214.0
140.90	781.0
142.90	878.0
144.80	375.0
148.00	198.0
154.70	184.0
156.80	196.0
171.90	712.0
172.90	671.0
173.90	61400.0
174.90	4408.0
175.90	57816.0
176.90	3751.0
178.00	285.0
206.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
36.00	473.0
36.90	2971.0
37.90	2829.0
38.90	1230.0
40.00	262.0
43.90	1014.0
44.80	537.0
46.80	933.0
47.80	319.0
48.90	2756.0
50.00	14082.0
50.90	4531.0
51.90	203.0
54.90	252.0
55.90	831.0
56.90	1825.0
60.00	717.0
60.90	3697.0
61.90	3988.0
62.90	3046.0
63.90	522.0
64.90	768.0
66.90	346.0
67.90	7586.0
68.90	8046.0
70.00	603.0
71.80	369.0
72.90	3454.0
74.00	13212.0
75.00	44232.0
75.90	3681.0
77.00	645.0
77.80	384.0
78.80	2676.0
79.90	888.0
80.80	2440.0
81.80	591.0
86.90	4194.0
87.90	3490.0
90.60	182.0
91.00	175.0
92.00	2095.0
92.90	3730.0
94.00	10083.0
95.00	88120.0
96.00	5350.0
103.90	376.0
104.90	155.0
105.80	410.0
115.80	305.0
116.90	657.0
117.70	405.0
118.90	452.0
128.00	338.0
128.80	127.0
129.80	328.0
130.80	118.0
134.70	251.0
137.00	250.0
140.90	995.0
142.80	975.0
144.80	362.0
148.00	180.0
149.70	148.0
154.70	259.0
156.90	188.0
171.90	834.0
172.80	655.0
173.90	68560.0
175.00	4875.0
175.90	65056.0
176.90	4178.0
178.00	349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
36.00	440.0
36.90	2979.0
37.80	2652.0
38.90	1233.0
39.90	239.0
43.90	977.0
44.90	540.0
46.80	852.0
47.80	277.0
48.90	2626.0
49.90	13825.0
50.90	4222.0
51.90	182.0
54.90	217.0
55.80	866.0
56.90	1902.0
60.00	628.0
60.90	3444.0
61.90	3881.0
62.90	2814.0
63.90	521.0
64.90	811.0
66.90	304.0
67.90	7643.0
68.90	7900.0
69.90	589.0
71.90	402.0
72.90	3398.0
74.00	12988.0
75.00	43136.0
75.90	3620.0
77.00	604.0
77.80	425.0
78.80	2521.0
79.90	815.0
80.80	2488.0
81.90	667.0
86.90	4141.0
87.90	3608.0
90.70	176.0
91.00	226.0
92.00	2140.0
92.90	3572.0
94.00	9836.0
95.00	87056.0
96.00	5346.0
96.90	148.0
103.90	377.0
104.90	161.0
105.80	453.0
110.70	114.0
115.70	240.0
116.90	572.0
117.80	370.0
118.90	460.0
123.70	130.0
128.00	324.0
128.80	165.0
129.80	443.0
130.80	110.0
134.70	224.0
136.60	171.0
137.00	233.0
140.90	1175.0
142.80	1042.0
144.80	382.0
145.80	111.0
147.90	199.0
149.70	158.0
154.70	275.0
157.00	166.0
171.90	802.0
172.80	622.0
173.90	69616.0
174.90	4875.0
175.90	66952.0
176.90	4161.0
178.00	289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069