


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111020\
 Data File : VU041193.D
 Acq On : 11 Nov 2020 09:11
 Operator : SY/MD
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 11 13:19:05 2020

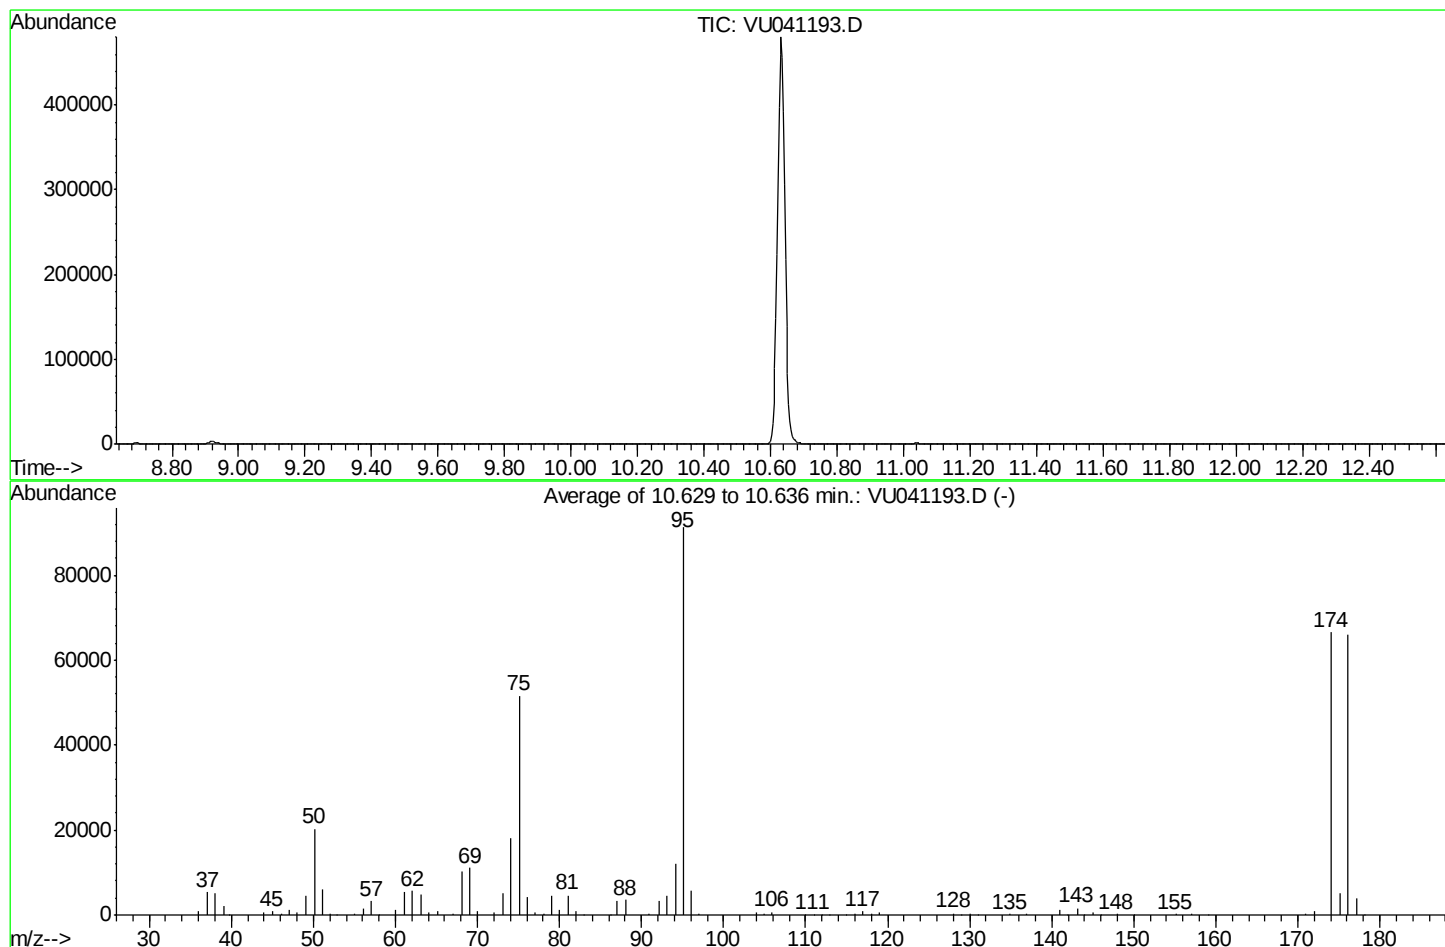

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	20202	PASS
75	95	30	80	56.5	51581	PASS
95	95	100	100	100.0	91264	PASS
96	95	5	9	6.4	5801	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.0	66589	PASS
175	174	5	9	7.5	5018	PASS
176	174	95	101	99.2	66082	PASS
177	176	5	9	6.0	3961	PASS

m/z	Abundance
36.00	962.0
37.10	5337.0
38.00	5310.0
39.10	2150.0
39.80	118.0
44.10	951.0
45.00	881.0
46.00	168.0
47.10	1303.0
48.00	641.0
49.10	4632.0
50.10	19976.0
51.10	6112.0
52.00	339.0
52.90	153.0
55.00	371.0
56.10	1622.0
57.10	3135.0
58.00	132.0
60.10	1188.0
61.10	5524.0
62.10	5637.0
63.10	4866.0
64.10	708.0
65.10	938.0
67.10	354.0
68.10	10194.0
69.10	10950.0
70.00	883.0
72.00	650.0
73.10	4940.0
74.10	18352.0
75.10	51400.0
76.10	4219.0
77.00	553.0
78.10	316.0
79.00	4556.0
79.90	1236.0
81.00	4479.0
82.00	976.0
82.90	145.0
87.00	3304.0
88.10	3575.0
90.90	421.0
92.10	3073.0
93.10	4629.0
94.10	11799.0
95.10	90536.0
96.10	5850.0
97.00	204.0
103.90	572.0
105.00	192.0
106.00	600.0
111.00	103.0
112.00	117.0
112.90	119.0
116.00	463.0
117.00	792.0
118.00	381.0
119.00	790.0
128.10	418.0
128.90	131.0
130.00	413.0
131.00	136.0
134.90	285.0
136.90	191.0
141.00	1146.0
141.90	125.0
143.10	1501.0
144.00	125.0
145.00	551.0
146.00	169.0
148.00	166.0
155.10	223.0
157.00	211.0
171.00	283.0
172.10	913.0
174.10	64448.0
175.10	5128.0
176.10	63568.0
177.10	3867.0
178.10	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1073.0
37.10	5569.0
38.00	5425.0
39.10	2268.0
39.80	111.0
44.10	892.0
45.00	903.0
46.10	174.0
47.10	1386.0
48.00	673.0
49.10	4673.0
50.10	20880.0
51.10	6290.0
52.00	305.0
52.90	130.0
55.00	432.0
56.10	1672.0
57.10	3329.0
58.00	136.0
60.00	1175.0
61.10	5436.0
62.10	5804.0
63.10	5024.0
64.10	677.0
65.10	930.0
67.10	373.0
68.10	10664.0
69.10	11403.0
70.00	981.0
72.00	688.0
73.10	5256.0
74.10	18376.0
75.10	53416.0
76.10	4444.0
77.00	602.0
78.00	353.0
79.00	4765.0
79.90	1276.0
81.00	4749.0
82.00	987.0
82.90	144.0
87.00	3538.0
88.10	3625.0
90.90	449.0
92.10	3392.0
93.10	4757.0
94.10	12562.0
95.10	94456.0
96.10	5976.0
97.10	207.0
104.00	538.0
105.00	193.0
106.00	620.0
110.00	100.0
111.00	130.0
112.90	116.0
114.90	115.0
115.90	477.0
117.00	860.0
118.00	393.0
119.00	769.0
128.00	464.0
129.00	147.0
130.00	441.0
131.00	112.0
134.90	314.0
136.90	200.0
141.00	1195.0
141.90	114.0
143.10	1579.0
144.00	112.0
145.00	526.0
146.00	156.0
148.00	164.0
150.00	105.0
155.10	225.0
157.00	187.0
171.00	268.0
172.10	879.0
174.10	68592.0
175.10	5154.0
176.10	68248.0
177.10	4039.0
178.10	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1070.0
37.10	5161.0
38.00	4910.0
39.10	2130.0
44.00	743.0
45.00	875.0
46.00	156.0
47.10	1161.0
48.00	673.0
49.10	4340.0
50.10	19752.0
51.10	5890.0
52.00	271.0
52.90	103.0
55.00	459.0
56.10	1684.0
57.10	3089.0
58.00	124.0
60.00	1043.0
61.10	5039.0
62.10	5332.0
63.10	4618.0
64.10	666.0
65.10	795.0
67.10	329.0
68.10	10255.0
69.10	10808.0
70.00	969.0
72.00	619.0
73.10	5005.0
74.10	17112.0
75.10	49928.0
76.10	4283.0
77.00	596.0
78.00	361.0
79.00	4449.0
80.00	1218.0
81.00	4568.0
82.00	978.0
83.00	115.0
86.20	132.0
87.00	3470.0
88.00	3320.0
91.00	438.0
92.10	3195.0
93.10	4422.0
94.10	11918.0
95.10	88800.0
96.10	5577.0
97.10	181.0
104.00	476.0
105.00	153.0
105.90	596.0
110.00	101.0
110.90	138.0
113.00	104.0
114.90	113.0
115.90	433.0
117.00	814.0
118.00	393.0
119.00	672.0
128.00	474.0
129.00	167.0
130.00	422.0
131.00	111.0
134.90	310.0
136.90	177.0
141.00	1135.0
141.90	107.0
143.10	1501.0
145.00	441.0
146.00	151.0
148.00	171.0
150.00	113.0
155.10	197.0
157.10	146.0
159.00	104.0
171.00	206.0
172.10	843.0
174.10	66728.0
175.10	4772.0
176.10	66432.0
177.10	3977.0
178.10	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
44.00	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10