
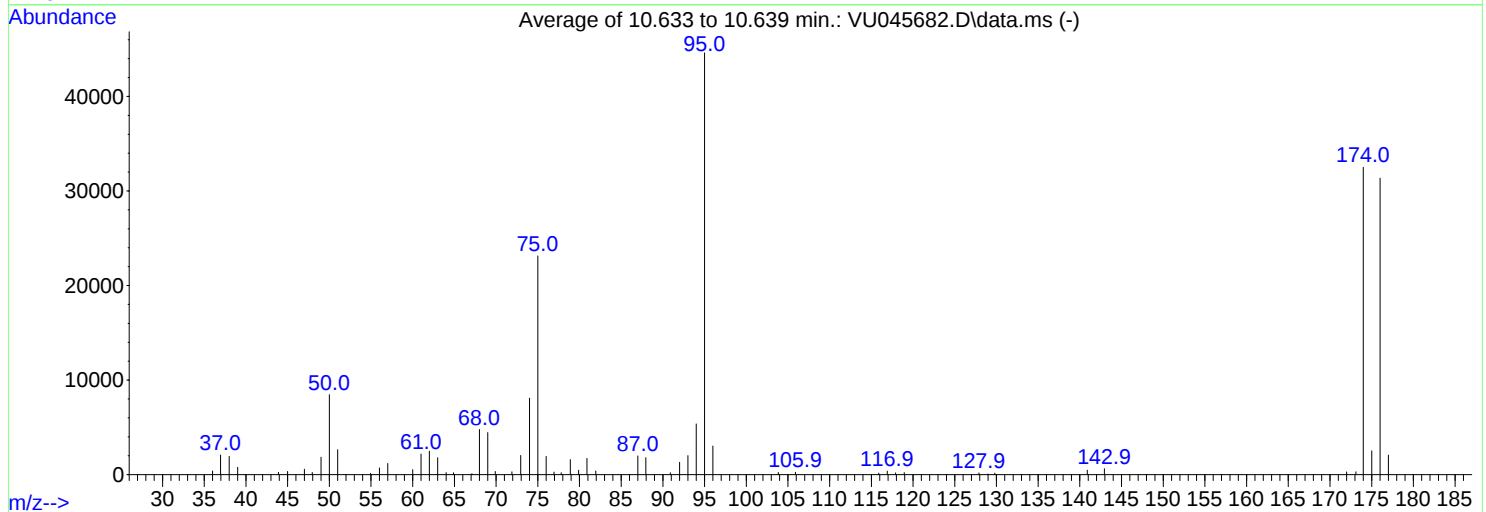


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111021\
 Data File : VU045682.D
 Acq On : 10 Nov 2021 09:34
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260
 Last Update : Fri Nov 05 13:35:16 2021

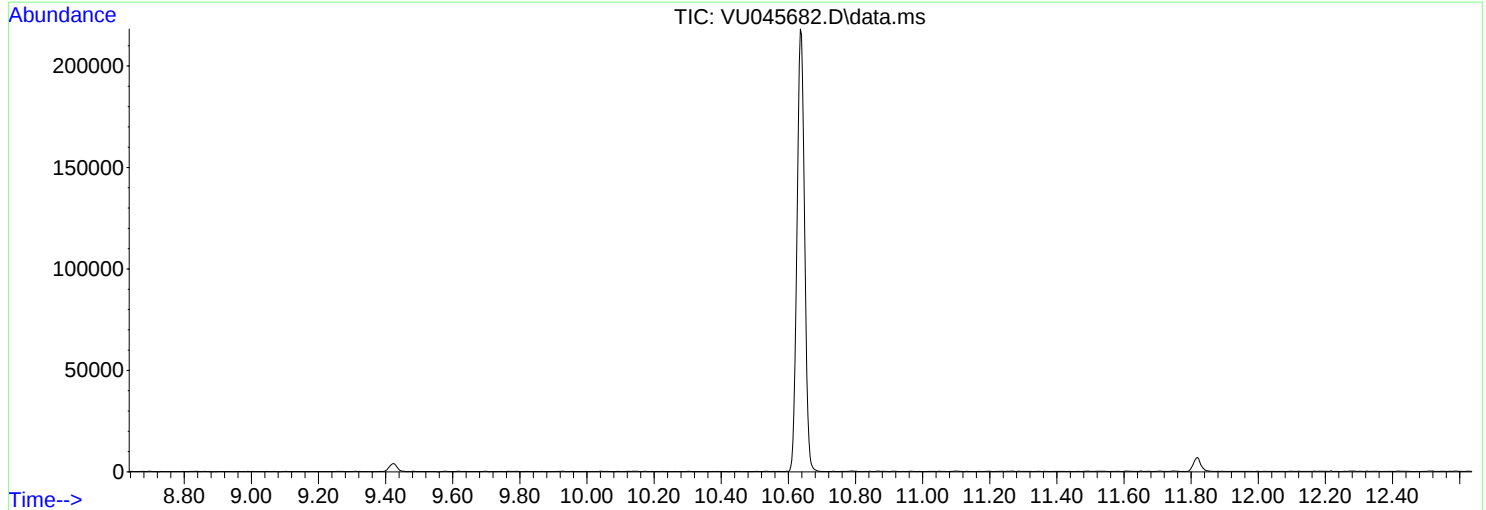

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	8462	PASS
75	95	30	60	51.8	23128	PASS
95	95	100	100	100.0	44611	PASS
96	95	5	9	6.8	3032	PASS
173	174	0.00	2	0.9	303	PASS
174	95	50	100	72.9	32512	PASS
175	174	5	9	7.7	2518	PASS
176	174	95	101	96.5	31360	PASS
177	176	5	9	6.6	2061	PASS