
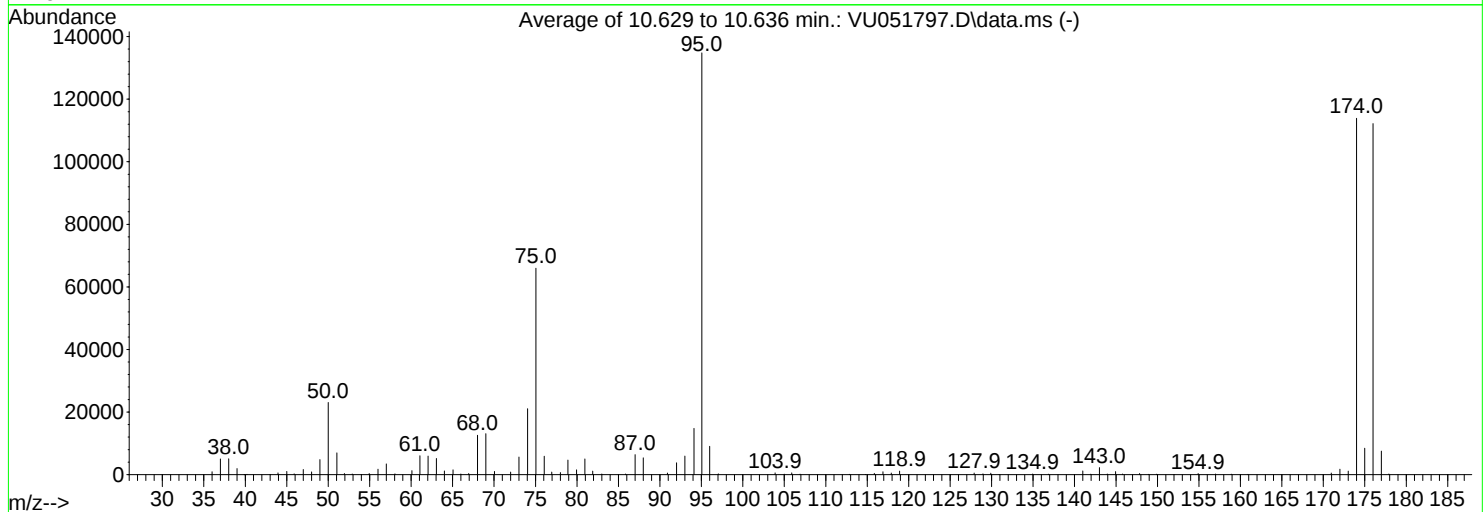


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111022\
 Data File : VU051797.D
 Acq On : 10 Nov 2022 09:22
 Operator : JC/MD
 Sample : BFB167
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB167

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 15 03:00:15 2022

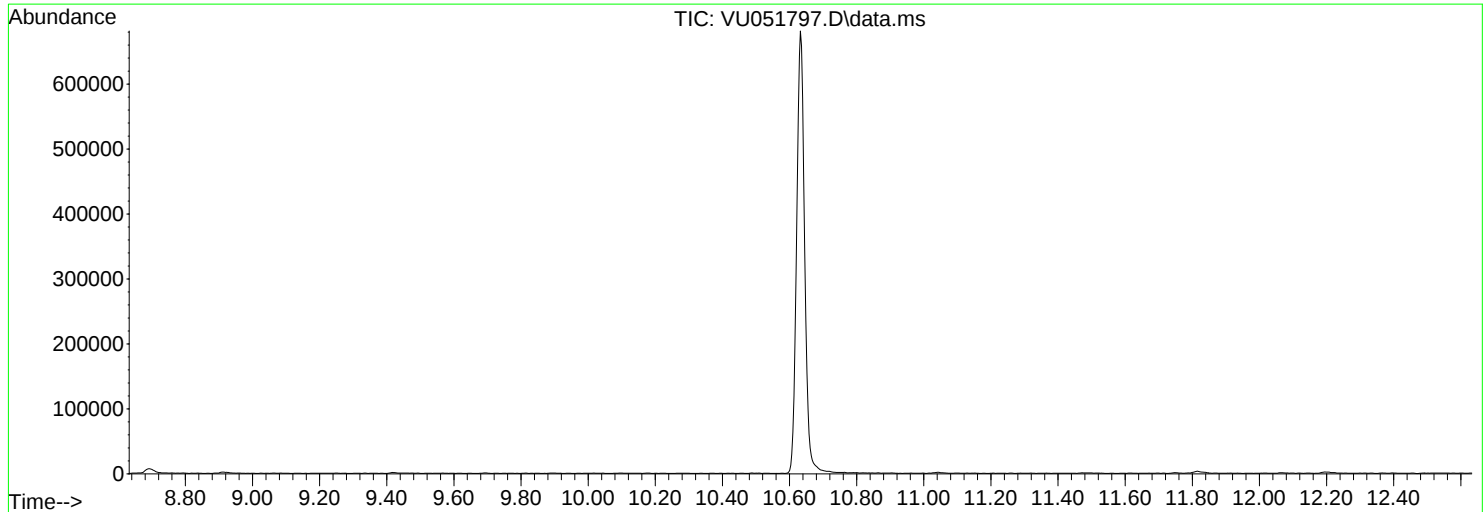

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	23059	PASS
75	95	30	80	48.9	65987	PASS
95	95	100	100	100.0	134805	PASS
96	95	5	9	6.7	9053	PASS
173	174	0.00	2	1.0	1144	PASS
174	95	50	120	84.5	113891	PASS
175	174	5	9	7.4	8461	PASS
176	174	95	101	98.5	112216	PASS
177	176	5	9	6.7	7521	PASS

m/z	Abundance
39.90	131.0
43.90	744.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.00	896.0
37.00	5023.0
38.00	4852.0
39.00	1955.0
40.20	251.0
43.00	129.0
44.00	1164.0
45.00	1044.0
45.90	272.0
47.00	1574.0
48.00	836.0
49.00	4590.0
50.00	23000.0
51.00	6951.0
51.90	390.0
52.90	206.0
54.00	100.0
54.90	335.0
56.00	1720.0
57.00	3479.0
58.00	254.0
60.10	1286.0
61.10	5788.0
62.00	5994.0
63.00	5200.0
64.00	1179.0
65.00	1613.0
66.00	211.0
67.00	381.0
68.00	12027.0
69.00	12911.0
70.00	1119.0
72.00	767.0
73.00	5646.0
74.10	20760.0
75.10	64608.0
76.10	5750.0
77.00	819.0
78.00	698.0
78.90	4761.0
79.90	1406.0
80.90	4993.0
81.90	1064.0
83.00	186.0
85.80	224.0
87.00	6199.0
88.00	5394.0
90.90	404.0
92.00	3809.0
93.00	5647.0
94.10	14327.0
95.10	131840.0
96.00	9067.0
97.00	272.0
103.90	527.0
105.00	125.0
105.90	623.0
106.90	136.0
112.80	107.0
115.90	355.0
116.90	852.0
117.90	541.0
118.90	1093.0
127.90	466.0
128.90	298.0
129.90	416.0
130.90	109.0
134.90	230.0
136.90	169.0
141.00	1192.0
141.90	158.0
143.00	2250.0
144.00	175.0
145.00	954.0
145.80	212.0
147.90	370.0
149.00	113.0
149.90	146.0
154.90	287.0
157.10	232.0
158.90	114.0
160.90	125.0
171.00	441.0
172.00	1697.0
173.00	1093.0
174.00	109704.0
175.00	8285.0
176.00	106528.0
177.00	7489.0
177.90	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.00	937.0
37.00	5178.0
38.00	5213.0
39.00	1981.0
39.90	216.0
44.00	1340.0
45.00	1075.0
45.90	281.0
47.00	1723.0
48.00	932.0
49.00	4914.0
50.00	23728.0
51.10	7223.0
52.00	411.0
52.90	205.0
54.90	337.0
56.00	1782.0
57.00	3590.0
58.00	239.0
60.10	1389.0
61.10	6193.0
62.10	6047.0
63.10	5189.0
64.00	1253.0
65.10	1594.0
66.00	186.0
67.00	357.0
68.00	12940.0
69.00	13542.0
70.00	1117.0
72.00	820.0
73.00	5765.0
74.00	21552.0
75.10	67912.0
76.10	6150.0
77.00	864.0
78.00	712.0
78.90	4776.0
80.00	1606.0
81.00	5234.0
81.90	1138.0
83.00	205.0
85.80	210.0
87.00	6694.0
88.00	5549.0
90.90	547.0
92.00	3905.0
93.00	6248.0
94.10	15294.0
95.10	138752.0
96.00	9449.0
97.00	242.0
103.90	608.0
105.00	161.0
105.90	584.0
106.90	150.0
112.80	145.0
115.90	404.0
116.90	943.0
117.90	522.0
118.90	1185.0
127.90	555.0
128.90	282.0
129.90	457.0
135.00	214.0
136.90	182.0
141.00	1252.0
142.00	184.0
143.00	2286.0
143.90	207.0
145.00	974.0
145.80	230.0
147.90	383.0
148.90	145.0
149.90	131.0
154.90	360.0
157.00	206.0
158.90	151.0
160.90	150.0
171.00	551.0
172.00	1827.0
173.00	1149.0
174.00	117512.0
175.00	8641.0
176.00	116104.0
177.00	7827.0
177.90	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167

m/z	Abundance
36.00	897.0
37.00	4788.0
38.00	5125.0
39.00	1852.0
39.80	217.0
44.00	1413.0
45.00	1027.0
45.90	245.0
47.00	1626.0
48.00	877.0
49.00	4917.0
50.00	22448.0
51.10	6758.0
52.00	365.0
52.90	198.0
55.00	385.0
56.00	1735.0
57.00	3240.0
58.10	211.0
60.10	1156.0
61.00	6081.0
62.00	5789.0
63.10	5059.0
64.00	1160.0
65.10	1451.0
66.00	168.0
66.90	340.0
68.00	12760.0
69.00	12810.0
70.10	895.0
72.00	847.0
73.00	5468.0
74.00	20872.0
75.00	65440.0
76.00	5747.0
76.90	822.0
78.00	651.0
78.90	4429.0
80.00	1662.0
81.00	4886.0
81.90	1143.0
83.00	173.0
85.90	182.0
87.00	6360.0
88.00	5198.0
90.90	620.0
92.00	3642.0
93.00	5955.0
94.10	14782.0
95.00	133824.0
96.00	8642.0
97.10	248.0
103.90	610.0
105.00	174.0
105.90	507.0
106.90	125.0
112.90	123.0
114.80	161.0
115.80	443.0
116.90	1043.0
117.90	474.0
118.90	1154.0
127.90	595.0
129.00	234.0
129.90	471.0
135.00	195.0
136.80	181.0
141.00	1167.0
142.00	146.0
143.00	2179.0
143.90	188.0
144.90	1008.0
145.80	189.0
147.80	361.0
148.90	136.0
149.90	135.0
152.00	109.0
154.90	378.0
156.90	216.0
158.90	158.0
160.90	121.0
170.90	559.0
172.00	1769.0
173.00	1189.0
174.00	114456.0
175.00	8456.0
176.00	114016.0
177.00	7248.0
177.90	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB167