

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
 Data File : VU056172.D
 Acq On : 10 Nov 2023 15:18
 Operator : MD/SY
 Sample : 05340-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDK9

Quant Time: Nov 10 22:21:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 10 22:17:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	359420	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	363050	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	163107	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	97967	4.391	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.800%
7) Chloroethane-d5	1.911	69	80185	5.296	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.000%
11) 1,1-Dichloroethene-d2	2.564	65	45698	4.649	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.000%
20) 2-Butanone-d5	4.621	46	265474	72.535	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	145.060%#
24) Chloroform-d	5.055	84	226108	5.324	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.400%
26) 1,2-Dichloroethane-d4	5.695	65	110338	5.901	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.000%
32) Benzene-d6	5.721	84	445786	5.112	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
36) 1,2-Dichloropropane-d6	6.686	67	140545	5.476	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%
41) Toluene-d8	7.895	98	385918	4.830	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	8.174	79	50542	5.151	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.000%
46) 2-Hexanone-d5	8.628	63	224350	69.766	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	139.540%#
56) 1,1,2,2-Tetrachloroeth...	10.750	84	110435	6.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.600%#
66) 1,2-Dichlorobenzene-d4	12.190	152	145933	5.802	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.000%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.576	96	5898	0.255	ug/L #	1
13) Acetone	2.637	43	30012	11.119	ug/L	99
17) Methyl tert-butyl Ether	3.358	73	20379	0.392	ug/L	98
19) 1,1-Dichloroethane	3.869	63	10727	0.240	ug/L	93
21) 2-Butanone	4.724	43	7192	1.616	ug/L	87
22) cis-1,2-Dichloroethene	4.660	96	18338	0.694	ug/L	92
27) 1,2-Dichloroethane	5.795	62	3816	0.142	ug/L #	91
34) Trichloroethene	6.538	95	552257	19.449	ug/L	97
47) Tetrachloroethene	8.550	164	198529	9.316	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
Data File : VU056172.D
Acq On : 10 Nov 2023 15:18
Operator : MD/SY
Sample : 05340-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDK9

Quant Time: Nov 10 22:21:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 10 22:17:51 2023
Response via : Initial Calibration

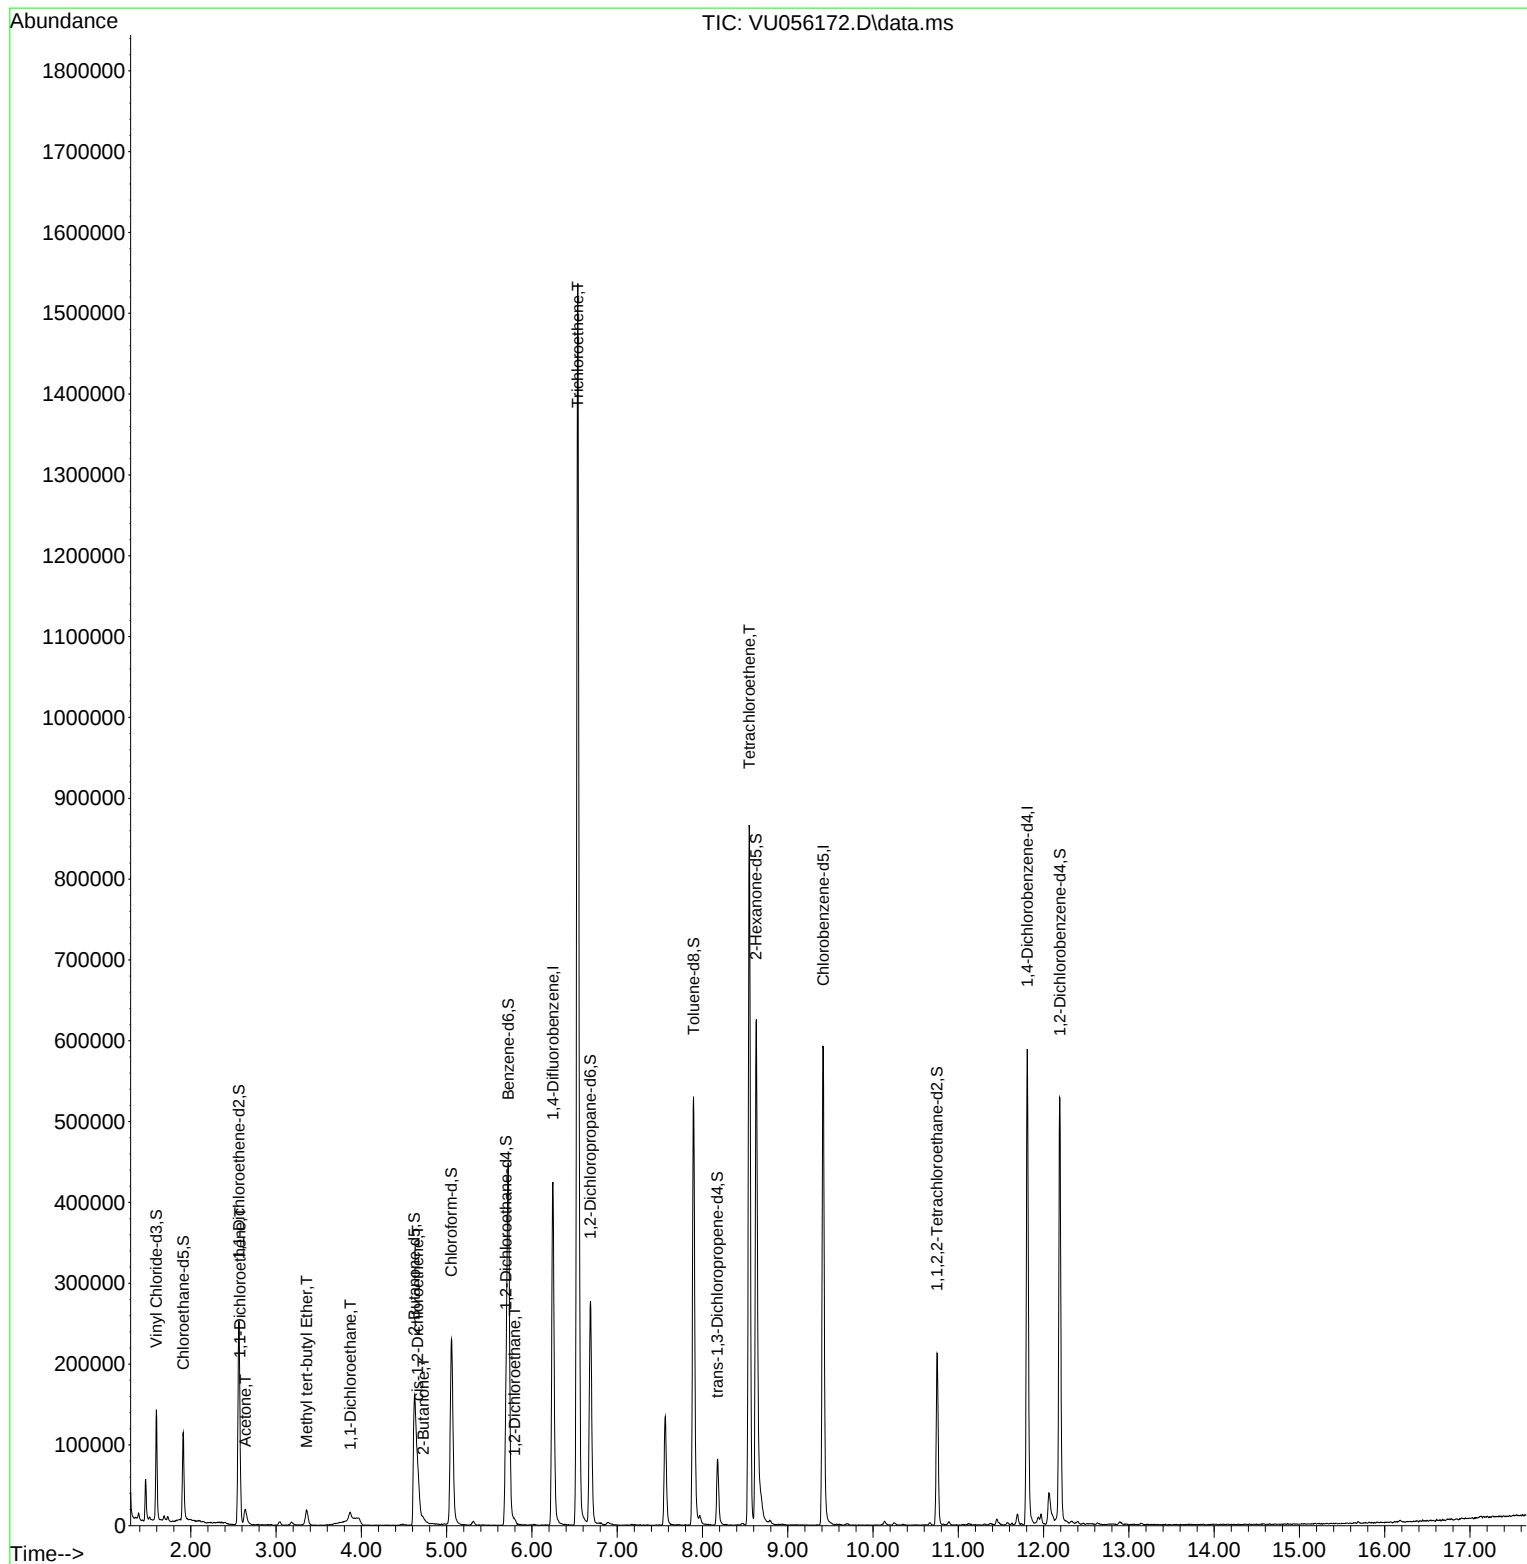

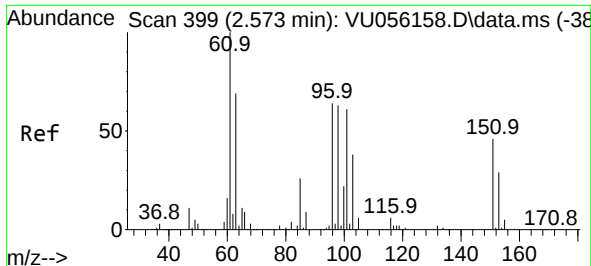

#12

1,1-Dichloroethene

Concen: 0.255 ug/L

RT: 2.576 min Scan# 400

Delta R.T. 0.003 min

Lab File: VU056172.D

Acq: 10 Nov 2023 15:18

Instrument :

MSVOA_U

ClientSampleId :

GCDK9





Tgt Ion: 96 Resp: 5898

Ion Ratio Lower Upper

96 100

61 284.5 111.7 207.5#

63 1397.5 74.5 138.3#

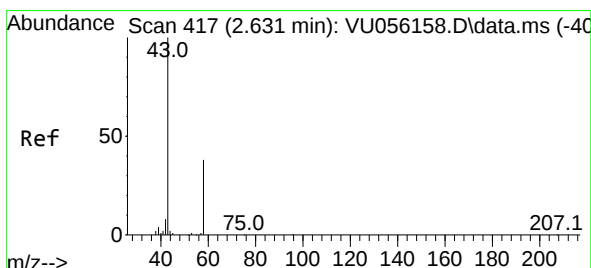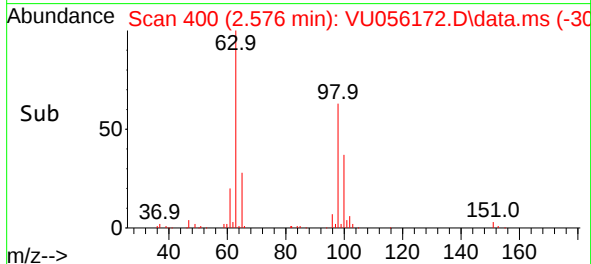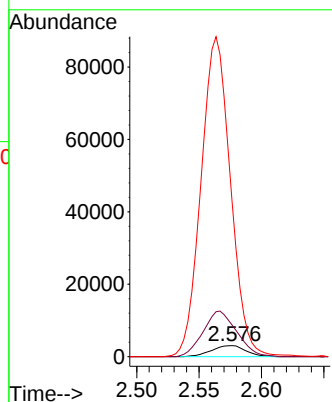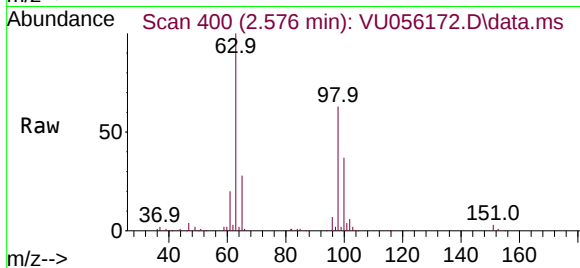

#13

Acetone

Concen: 11.119 ug/L

RT: 2.637 min Scan# 419

Delta R.T. 0.006 min

Lab File: VU056172.D




Acq: 10 Nov 2023 15:18


Tgt Ion: 43 Resp: 30012

Ion Ratio Lower Upper

43 100

58 38.0 0.0 74.4

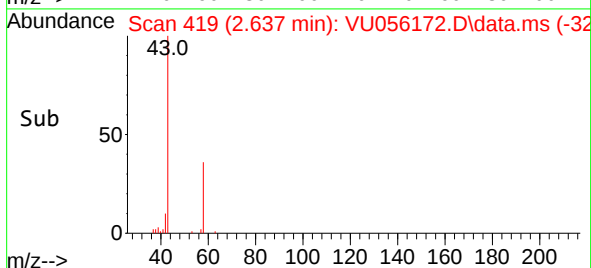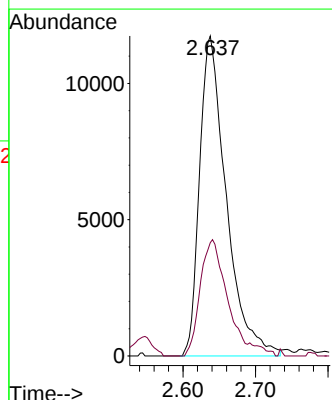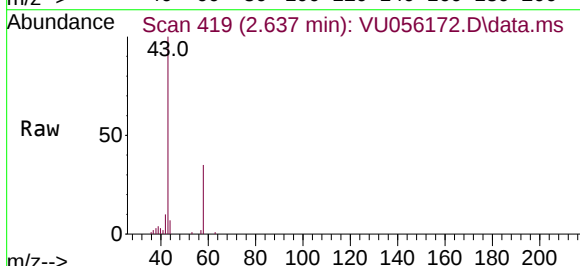

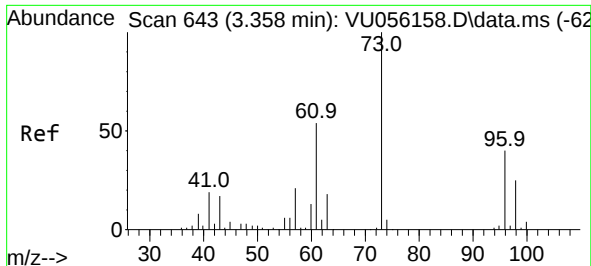

#17

Methyl tert-butyl Ether

Concen: 0.392 ug/L

RT: 3.358 min Scan# 643

Delta R.T. 0.000 min

Lab File: VU056172.D

Acq: 10 Nov 2023 15:18

Instrument :

MSVOA_U

ClientSampleId :

GCDK9





Tgt Ion: 73 Resp: 20379

Ion Ratio Lower Upper

73 100

43 19.0 13.6 20.4

57 21.9 17.3 25.9

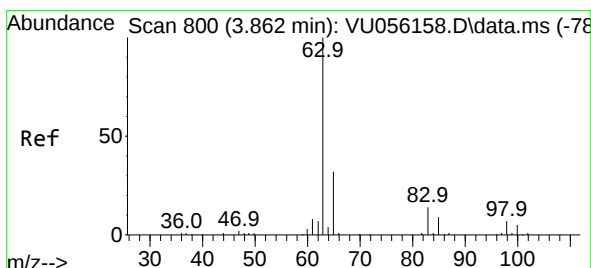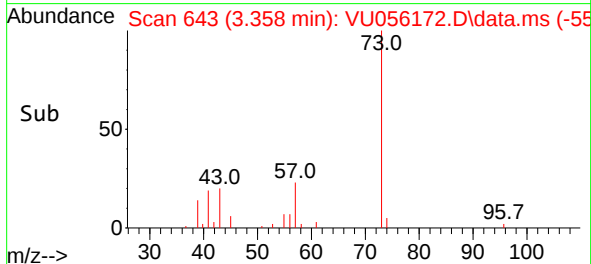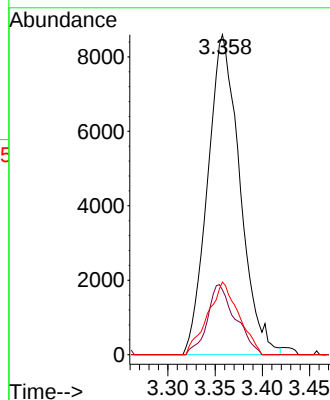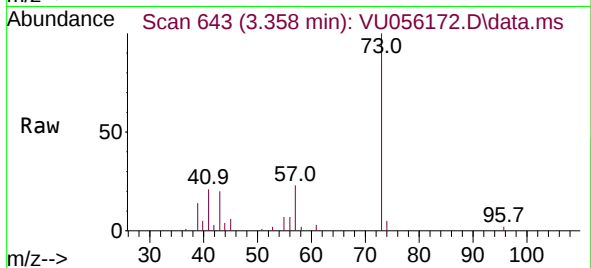

#19

1,1-Dichloroethane

Concen: 0.240 ug/L

RT: 3.869 min Scan# 802

Delta R.T. 0.006 min

Lab File: VU056172.D

Acq: 10 Nov 2023 15:18




Tgt Ion: 63 Resp: 10727


Ion Ratio Lower Upper

63 100

65 33.3 20.6 38.2

83 16.2 9.6 17.8


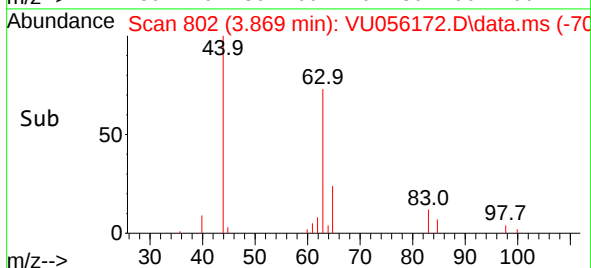
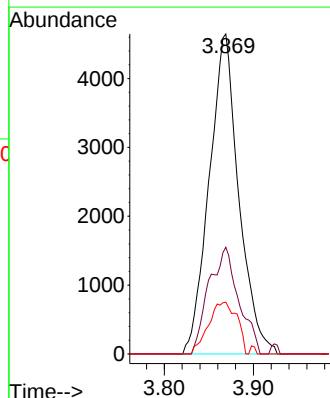
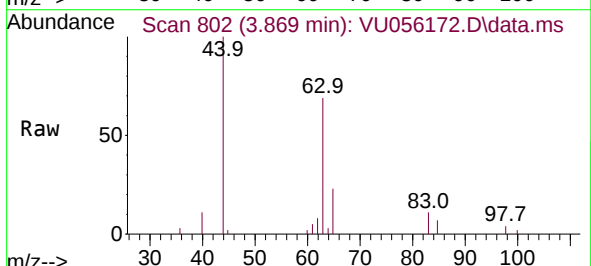


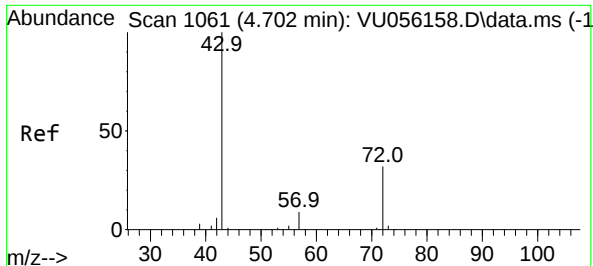

#21
2-Butanone
Concen: 1.616 ug/L
RT: 4.724 min Scan# 1068
Delta R.T. 0.023 min
Lab File: VU056172.D
Acq: 10 Nov 2023 15:18




Instrument :
MSVOA_U
ClientSampleId :
GCDK9


Tgt Ion: 43 Resp: 7192
Ion Ratio Lower Upper
43 100
72 38.8 15.7 47.0

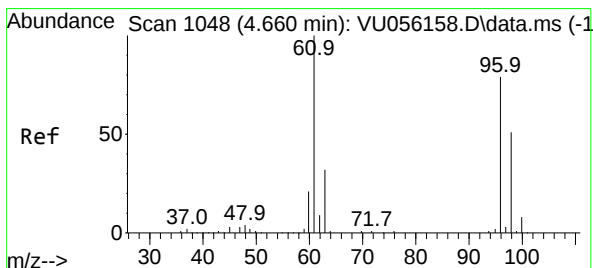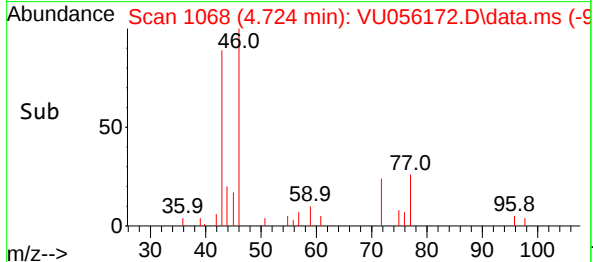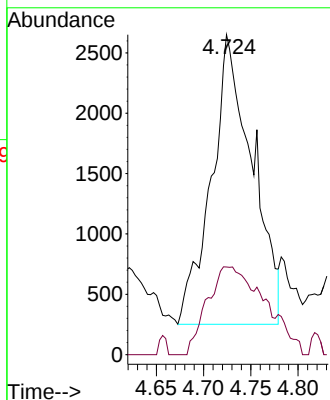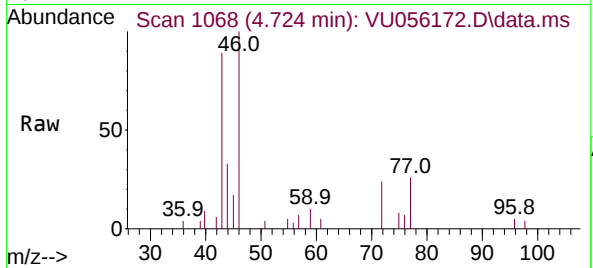

#22
cis-1,2-Dichloroethene
Concen: 0.694 ug/L
RT: 4.660 min Scan# 1048
Delta R.T. 0.000 min
Lab File: VU056172.D
Acq: 10 Nov 2023 15:18

Tgt Ion: 96 Resp: 18338
Ion Ratio Lower Upper
96 100
61 139.2 87.8 163.2
98 62.4 43.5 80.7


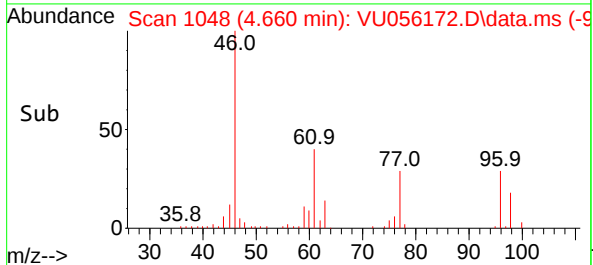
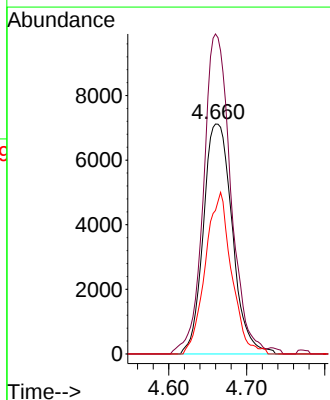
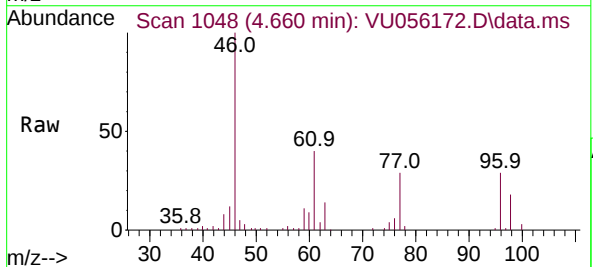


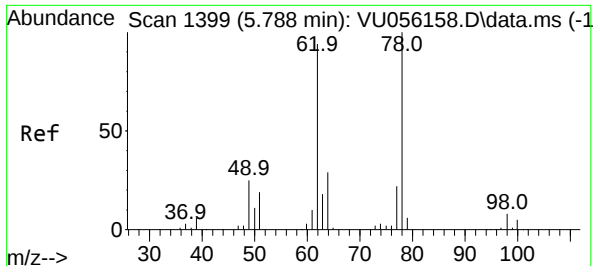

#27
1,2-Dichloroethane
Concen: 0.142 ug/L
RT: 5.795 min Scan# 1401
Delta R.T. 0.006 min
Lab File: VU056172.D
Acq: 10 Nov 2023 15:18




Instrument :
MSVOA_U
ClientSampleId :
GCDK9


Tgt Ion: 62 Resp: 3816
Ion Ratio Lower Upper
62 100
98 12.0 7.1 10.7#

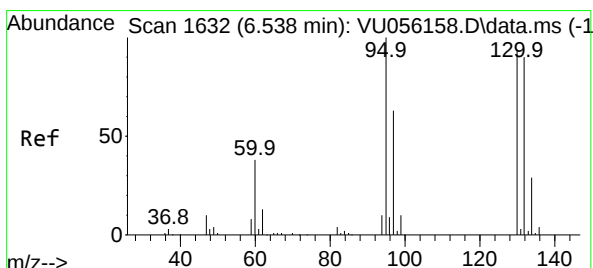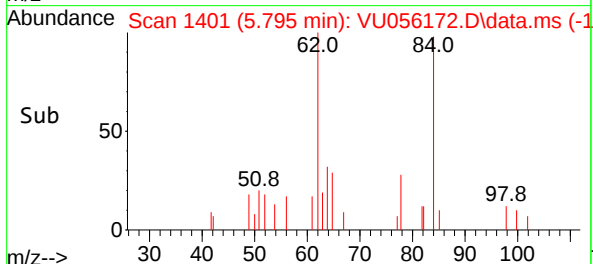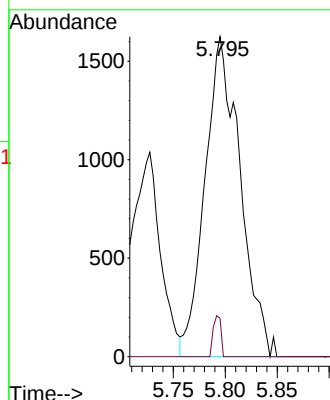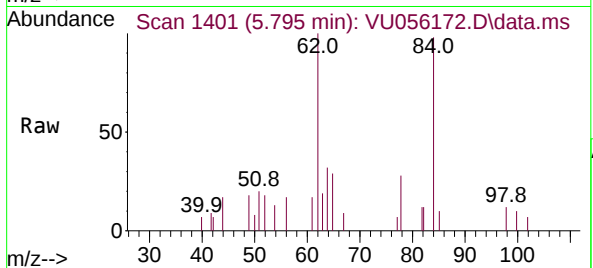

#34
Trichloroethene
Concen: 19.449 ug/L
RT: 6.538 min Scan# 1632
Delta R.T. 0.000 min
Lab File: VU056172.D
Acq: 10 Nov 2023 15:18

Tgt Ion: 95 Resp: 552257
Ion Ratio Lower Upper
95 100
97 65.0 46.8 87.0
132 92.2 66.5 123.5
130 96.6 70.6 131.0

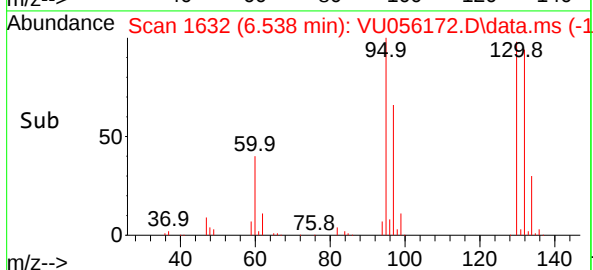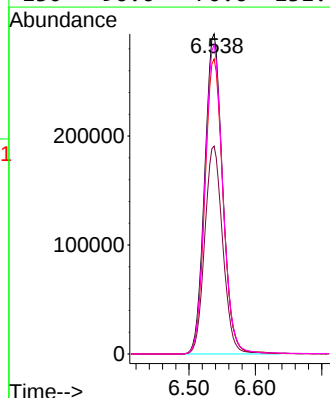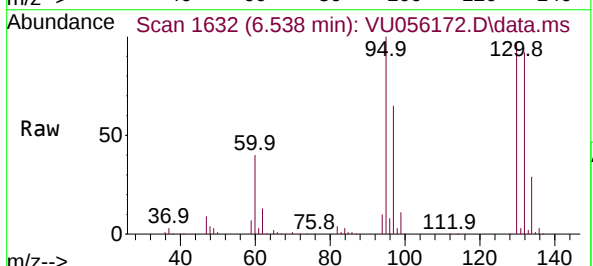

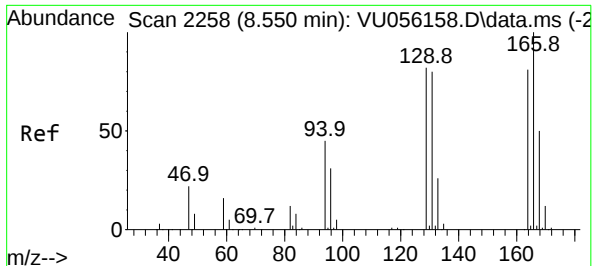

#47
 Tetrachloroethene
 Concen: 9.316 ug/L
 RT: 8.550 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VU056172.D
 Acq: 10 Nov 2023 15:18

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDK9

Tgt Ion:164 Resp: 198529

Ion	Ratio	Lower	Upper
164	100		
129	97.9	66.6	123.8
131	94.2	67.8	126.0
166	126.5	85.9	159.5

