

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
 Data File : VU056179.D
 Acq On : 10 Nov 2023 18:57
 Operator : MD/SY
 Sample : 05340-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDL1

Quant Time: Nov 11 01:41:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 11 00:40:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	375363	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	372041	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	176707	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	101368	4.351	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.000%
7) Chloroethane-d5	1.907	69	83217	5.263	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.200%
11) 1,1-Dichloroethene-d2	2.563	65	48844	4.758	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.200%
20) 2-Butanone-d5	4.618	46	276248	72.273	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	144.540%#
24) Chloroform-d	5.058	84	234560	5.289	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.800%
26) 1,2-Dichloroethane-d4	5.695	65	110807	5.674	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.400%
32) Benzene-d6	5.721	84	464644	5.200	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.000%
36) 1,2-Dichloropropane-d6	6.685	67	144043	5.476	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%
41) Toluene-d8	7.894	98	388069	4.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	8.177	79	51069	5.079	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.600%
46) 2-Hexanone-d5	8.627	63	237463	72.059	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	144.120%#
56) 1,1,2,2-Tetrachloroeth...	10.753	84	112953	6.017	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.400%#
66) 1,2-Dichlorobenzene-d4	12.190	152	151572	5.562	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	29651	10.519	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
Data File : VU056179.D
Acq On : 10 Nov 2023 18:57
Operator : MD/SY
Sample : 05340-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDL1

Quant Time: Nov 11 01:41:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 11 00:40:59 2023
Response via : Initial Calibration

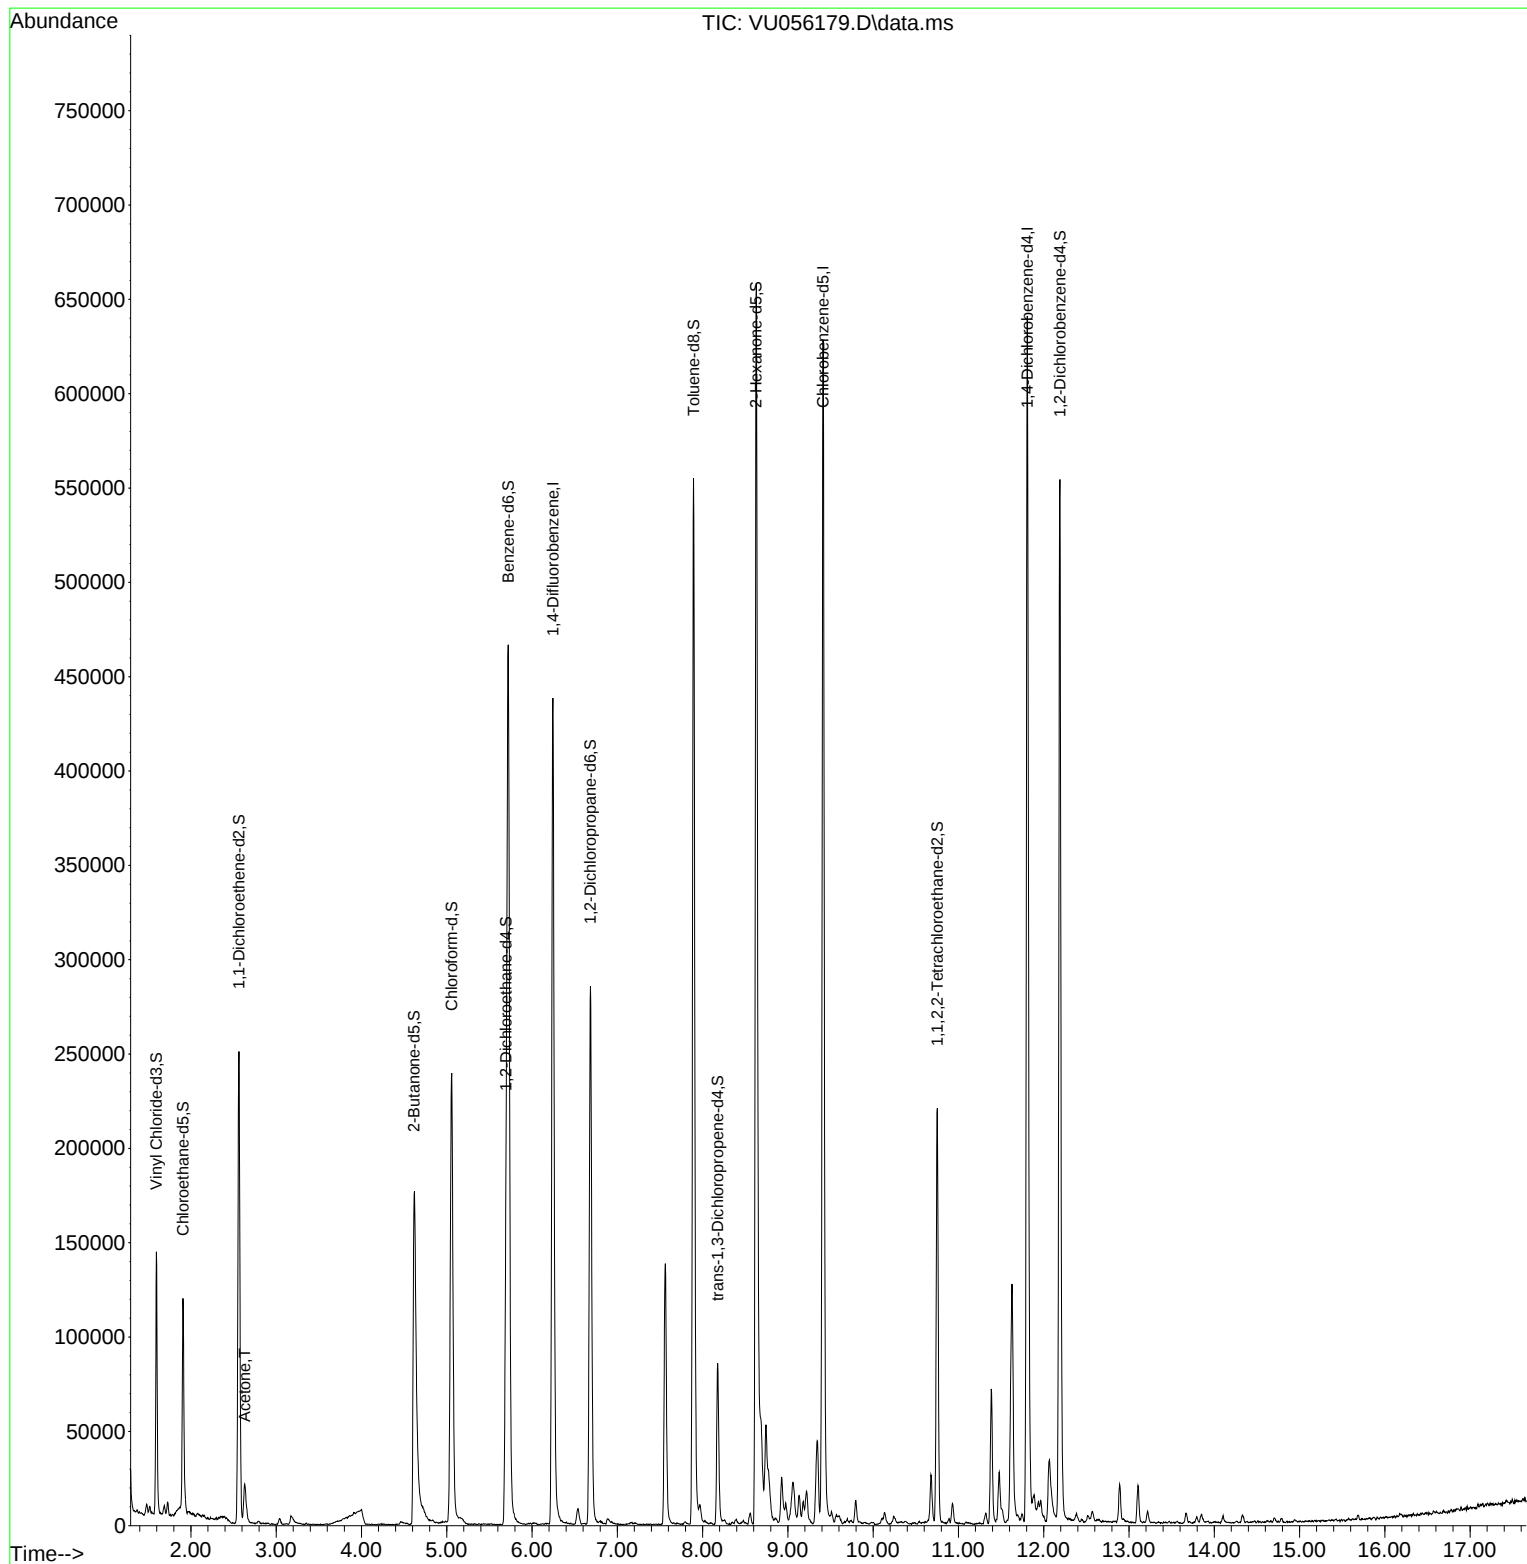

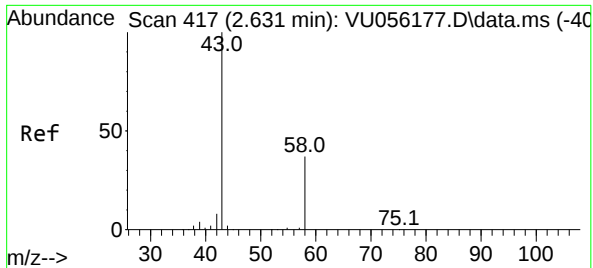

#13
 Acetone
 Concen: 10.519 ug/L
 RT: 2.631 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU056179.D
 Acq: 10 Nov 2023 18:57

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDL1

Tgt Ion: 43 Resp: 29651
 Ion Ratio Lower Upper
 43 100
 58 33.3 0.0 74.4

