

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
 Data File : VU056191.D
 Acq On : 10 Nov 2023 23:49
 Operator : MD/SY
 Sample : 05339-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDJ1

Quant Time: Nov 11 01:44:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 11 00:40:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Difluorobenzene	6.245	114	366048	5.000 ug/L	0.00
28) Chlorobenzene-d5	9.415	117	367748	5.000 ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	165582	5.000 ug/L	0.00
System Monitoring Compounds					
4) Vinyl Chloride-d3	1.596	65	98149	4.320 ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 86.400%	
7) Chloroethane-d5	1.907	69	79316	5.144 ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 102.800%	
11) 1,1-Dichloroethene-d2	2.563	65	45154	4.511 ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 90.200%	
20) 2-Butanone-d5	4.621	46	277930	74.563 ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 149.120%#	
24) Chloroform-d	5.055	84	227193	5.253 ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 105.000%	
26) 1,2-Dichloroethane-d4	5.698	65	110738	5.815 ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 116.200%	
32) Benzene-d6	5.721	84	451105	5.107 ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 102.200%	
36) 1,2-Dichloropropane-d6	6.685	67	142199	5.469 ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 109.400%	
41) Toluene-d8	7.894	98	379508	4.689 ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 93.800%	
43) trans-1,3-Dichloroprop...	8.177	79	48918	4.922 ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 98.400%	
46) 2-Hexanone-d5	8.627	63	226973	69.680 ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 139.360%#	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	110577	5.959 ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 119.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152	143148	5.606 ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 112.200%	
Target Compounds					
13) Acetone	2.637	43	20377	7.413 ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
Data File : VU056191.D
Acq On : 10 Nov 2023 23:49
Operator : MD/SY
Sample : 05339-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDJ1

Quant Time: Nov 11 01:44:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 11 00:40:59 2023
Response via : Initial Calibration

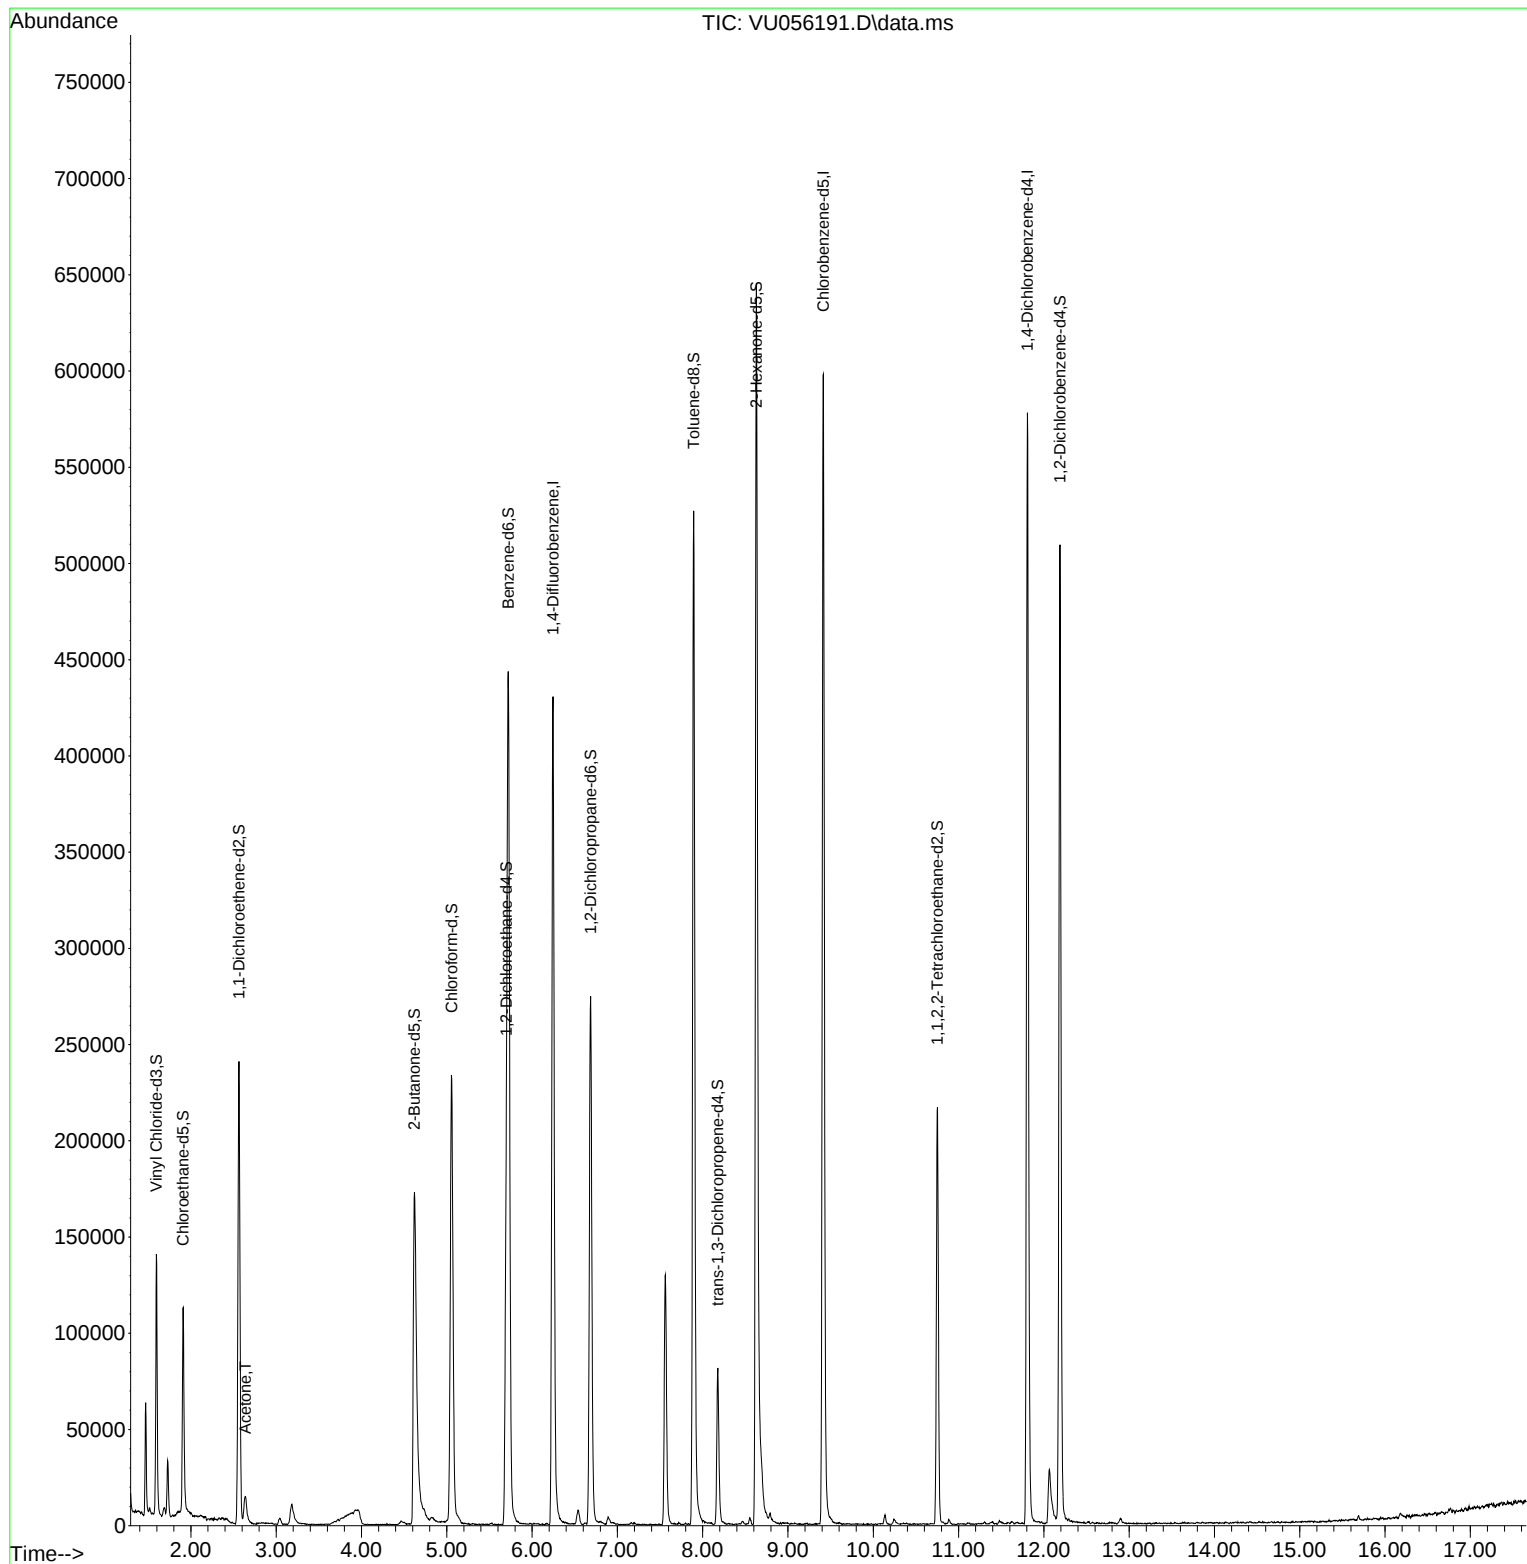

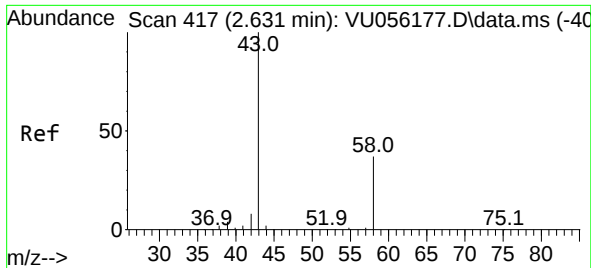

#13
 Acetone
 Concen: 7.413 ug/L
 RT: 2.637 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VU056191.D
 Acq: 10 Nov 2023 23:49

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDJ1

Tgt Ion: 43 Resp: 20377
 Ion Ratio Lower Upper
 43 100
 58 40.3 0.0 74.4

