

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111023\  
 Data File : VU056192.D  
 Acq On : 11 Nov 2023 00:13  
 Operator : MD/SY  
 Sample : 05339-07  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 34 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCDJ2

Quant Time: Nov 11 01:44:36 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR110723WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Nov 11 00:40:59 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units     | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|-----------|----------|
| -----                         |        |                |          |        |           |          |
| Internal Standards            |        |                |          |        |           |          |
| 1) 1,4-Difluorobenzene        | 6.245  | 114            | 363743   | 5.000  | ug/L      | 0.00     |
| 28) Chlorobenzene-d5          | 9.415  | 117            | 366174   | 5.000  | ug/L      | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.807 | 152            | 160634   | 5.000  | ug/L      | 0.00     |
| System Monitoring Compounds   |        |                |          |        |           |          |
| 4) Vinyl Chloride-d3          | 1.596  | 65             | 98280    | 4.353  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 87.000%   |          |
| 7) Chloroethane-d5            | 1.908  | 69             | 79617    | 5.196  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 104.000%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.563  | 65             | 45395    | 4.564  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 91.200%   |          |
| 20) 2-Butanone-d5             | 4.621  | 46             | 270385   | 72.999 | ug/L      | 0.00     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 146.000%# |          |
| 24) Chloroform-d              | 5.055  | 84             | 229165   | 5.332  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 106.600%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.695  | 65             | 108730   | 5.746  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 115.000%  |          |
| 32) Benzene-d6                | 5.721  | 84             | 443444   | 5.042  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 100.800%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.685  | 67             | 140485   | 5.427  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 108.600%  |          |
| 41) Toluene-d8                | 7.894  | 98             | 379543   | 4.710  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 94.200%   |          |
| 43) trans-1,3-Dichloroprop... | 8.177  | 79             | 48152    | 4.866  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 97.400%   |          |
| 46) 2-Hexanone-d5             | 8.631  | 63             | 219395   | 67.643 | ug/L      | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 135.280%# |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.753 | 84             | 111925   | 6.057  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 121.200%# |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.190 | 152            | 145851   | 5.888  | ug/L      | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 117.800%  |          |
| Target Compounds              |        |                |          |        |           |          |
|                               |        |                |          |        | Qvalue    |          |
| 13) Acetone                   | 2.631  | 43             | 50178    | 18.369 | ug/L      | 98       |
| -----                         |        |                |          |        |           |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111023\  
Data File : VU056192.D  
Acq On : 11 Nov 2023 00:13  
Operator : MD/SY  
Sample : 05339-07  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
GCDJ2

Quant Time: Nov 11 01:44:36 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR110723WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Nov 11 00:40:59 2023  
Response via : Initial Calibration

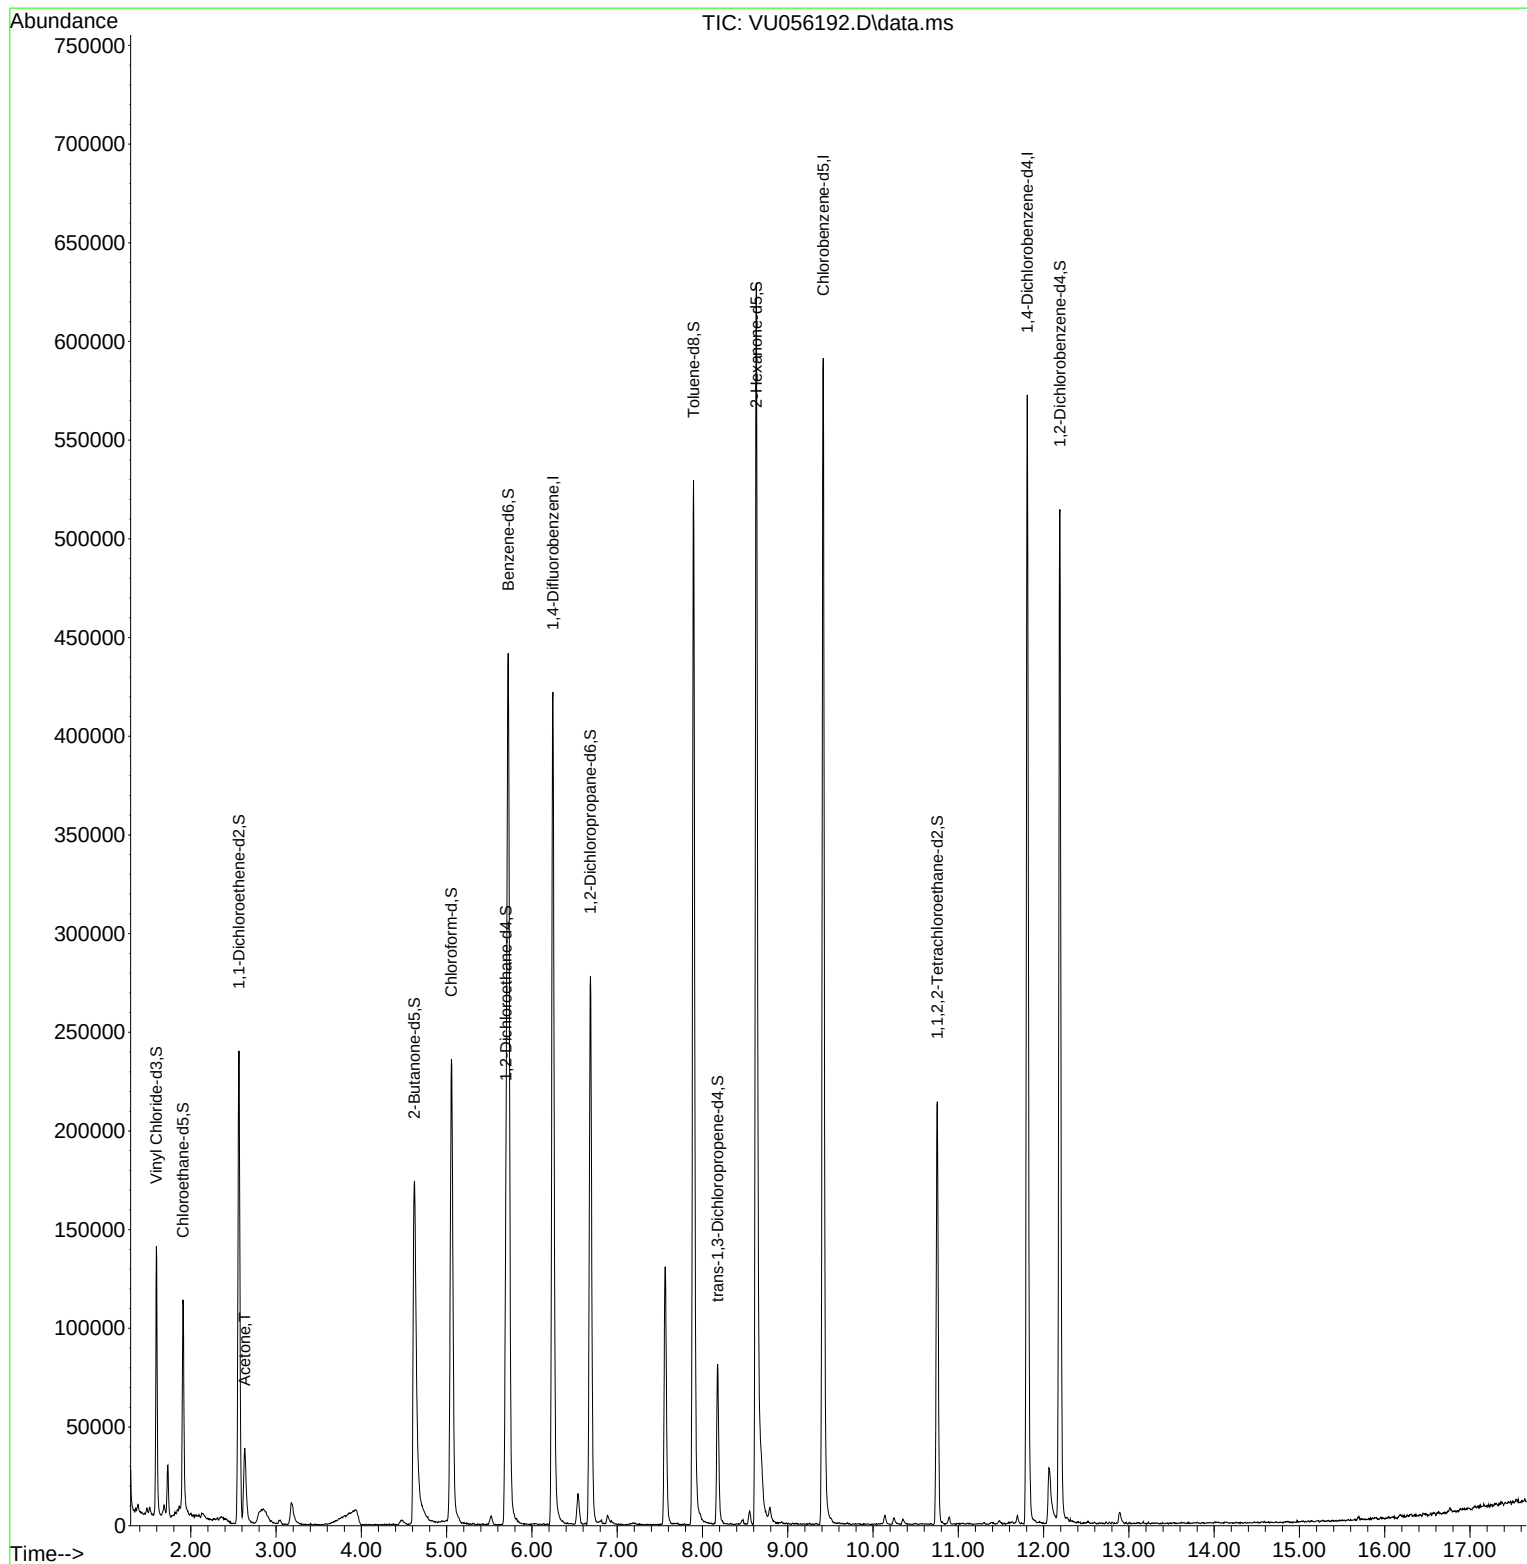

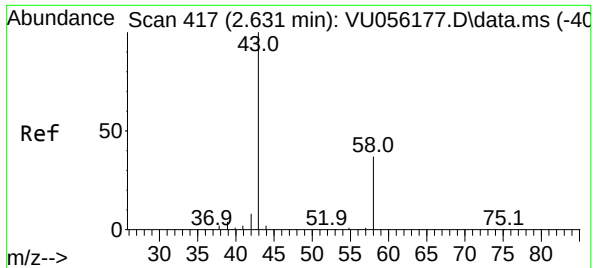

#13  
 Acetone  
 Concen: 18.369 ug/L  
 RT: 2.631 min Scan# 41  
 Delta R.T. 0.000 min  
 Lab File: VU056192.D  
 Acq: 11 Nov 2023 00:13

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCDJ2

Tgt Ion: 43 Resp: 50178  
 Ion Ratio Lower Upper  
 43 100  
 58 36.3 0.0 74.4

