


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111023\
Data File : VU056157.D
Acq On : 10 Nov 2023 08:24
Operator : MD/SY
Sample : BFB070
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB070

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR110723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 11 22:15:12 2023

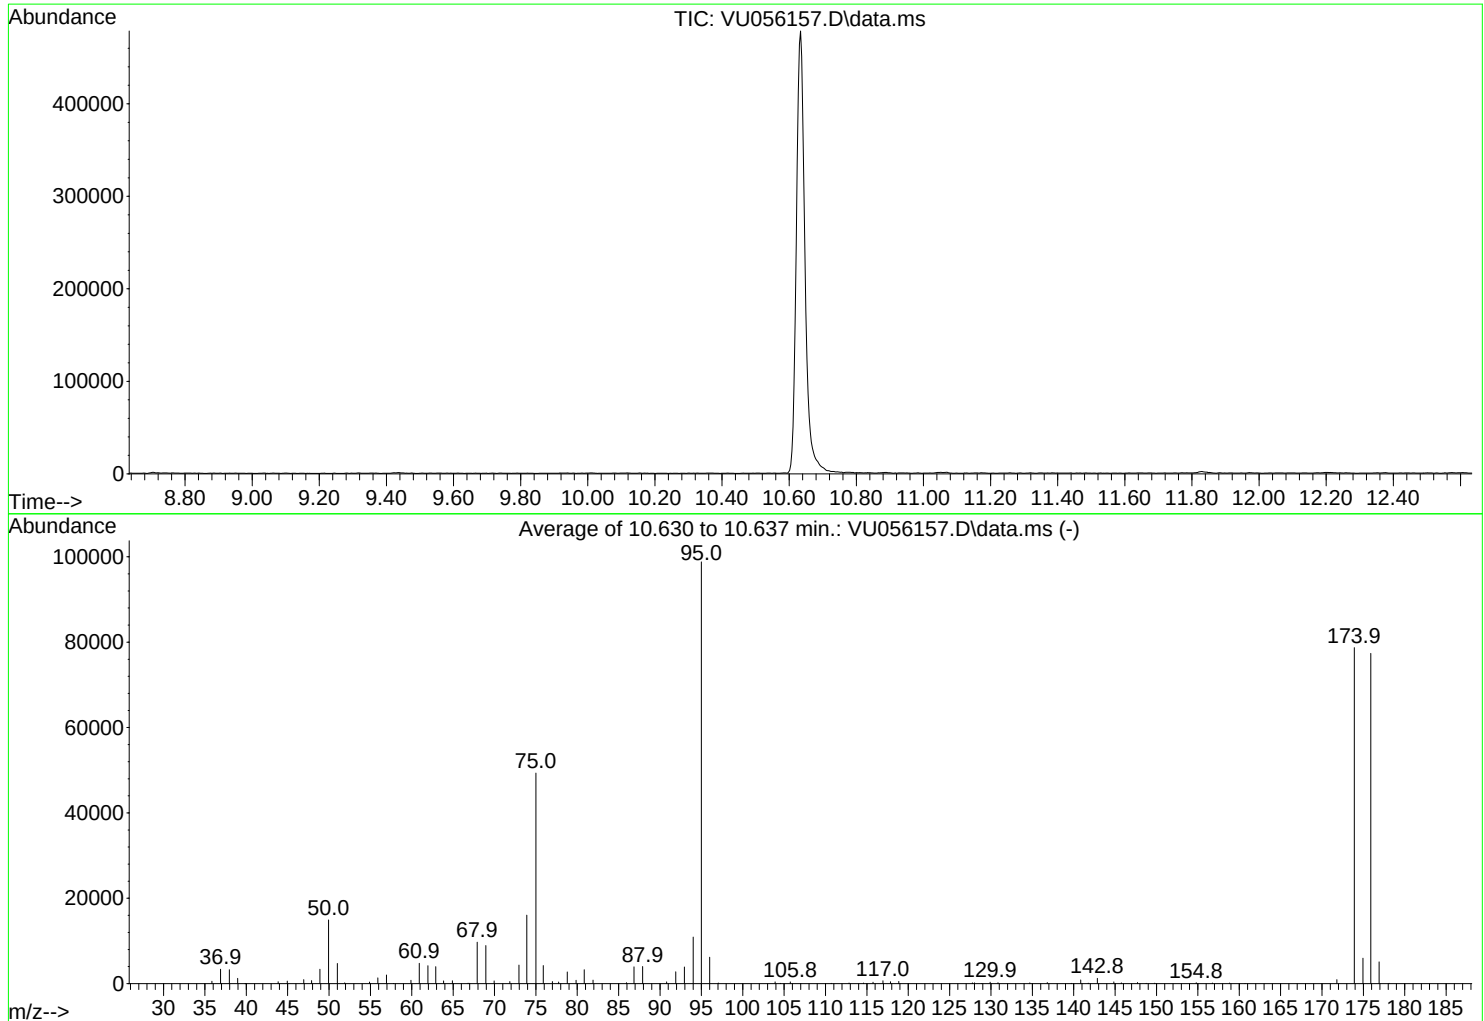

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	14926	PASS
75	95	30	80	49.9	49339	PASS
95	95	100	100	100.0	98821	PASS
96	95	5	9	6.3	6204	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.7	78739	PASS
175	174	5	9	7.6	5971	PASS
176	174	95	101	98.2	77357	PASS
177	176	5	9	6.6	5095	PASS

m/z	Abundance
39.80	287.0
43.00	127.0
43.80	633.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	607.0
36.90	3295.0
37.90	3161.0
39.00	1318.0
39.90	291.0
43.90	1123.0
45.00	535.0
47.00	1001.0
47.90	754.0
48.90	3330.0
49.90	15283.0
51.00	4819.0
51.90	226.0
54.90	373.0
55.90	1357.0
56.90	2093.0
57.80	111.0
59.90	748.0
60.90	4945.0
62.00	4185.0
62.90	4108.0
63.90	687.0
64.90	623.0
66.80	216.0
67.90	9273.0
68.90	8814.0
69.90	573.0
71.90	486.0
72.90	4224.0
73.90	16163.0
75.00	49488.0
75.90	4463.0
77.00	541.0
77.70	313.0
78.80	2785.0
79.80	762.0
80.90	3134.0
81.90	761.0
86.00	200.0
86.80	3834.0
87.90	4160.0
90.80	418.0
91.90	2847.0
93.00	3843.0
94.00	11124.0
95.00	99608.0
96.00	6522.0
97.10	147.0
103.90	374.0
105.80	465.0
110.70	104.0
112.90	123.0
114.60	156.0
115.70	383.0
116.90	602.0
117.80	428.0
118.90	482.0
128.00	319.0
128.90	100.0
129.90	344.0
130.80	187.0
134.70	246.0
136.80	298.0
139.70	100.0
140.90	842.0
141.70	109.0
142.80	1258.0
144.80	333.0
145.70	185.0
147.70	236.0
148.80	115.0
149.80	153.0
154.80	227.0
156.70	166.0
158.90	178.0
160.70	116.0
171.80	967.0
173.90	77928.0
175.00	5888.0
175.90	76272.0
176.90	5058.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.80	585.0
36.90	3431.0
37.90	3403.0
38.90	1241.0
40.00	282.0
44.00	1104.0
45.00	602.0
46.90	923.0
47.90	761.0
48.90	3463.0
49.90	15314.0
51.00	4818.0
51.90	195.0
54.90	385.0
55.90	1401.0
57.00	2040.0
59.90	837.0
60.90	4902.0
61.90	4340.0
62.90	4205.0
63.90	652.0
64.90	663.0
66.80	175.0
67.90	10085.0
68.90	9243.0
69.90	644.0
71.80	487.0
73.00	4430.0
73.90	16552.0
75.00	50752.0
75.90	4296.0
77.00	504.0
77.70	389.0
78.80	2860.0
79.90	782.0
80.80	3388.0
81.90	822.0
85.90	215.0
86.80	4089.0
87.90	4202.0
90.80	470.0
91.90	2811.0
93.00	3946.0
94.00	11287.0
95.00	101712.0
96.00	6246.0
97.10	151.0
103.90	432.0
104.50	122.0
105.70	461.0
110.70	116.0
112.90	154.0
114.60	155.0
115.80	340.0
117.00	689.0
117.80	480.0
118.90	520.0
127.70	263.0
128.00	277.0
129.90	359.0
130.90	248.0
134.70	204.0
136.80	297.0
139.70	100.0
140.80	895.0
141.80	119.0
142.80	1309.0
144.80	408.0
145.80	223.0
147.70	251.0
148.70	123.0
149.80	127.0
154.80	208.0
156.80	151.0
158.80	160.0
171.80	981.0
173.90	80992.0
174.90	6210.0
175.90	79792.0
176.90	5267.0
178.10	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.80	545.0
36.90	3401.0
38.00	3254.0
38.90	1135.0
40.00	292.0
44.00	1064.0
44.90	621.0
46.90	914.0
47.90	618.0
48.90	3373.0
50.00	14182.0
51.00	4524.0
51.90	168.0
54.90	333.0
55.90	1310.0
57.00	1986.0
59.90	776.0
60.90	4464.0
61.90	4118.0
62.90	3630.0
63.80	549.0
64.90	715.0
67.00	183.0
67.90	9831.0
69.00	8733.0
70.00	698.0
71.80	485.0
73.00	4386.0
73.90	15375.0
75.00	47776.0
75.90	3912.0
77.00	470.0
77.80	443.0
78.80	2604.0
79.90	775.0
80.80	3326.0
81.90	846.0
86.00	211.0
86.90	3880.0
87.90	3731.0
90.80	398.0
91.90	2625.0
92.90	3898.0
94.00	10306.0
95.00	95144.0
96.00	5844.0
97.00	165.0
103.90	423.0
104.60	142.0
105.80	370.0
107.00	107.0
112.80	141.0
114.60	103.0
115.80	291.0
117.00	781.0
117.90	467.0
118.80	526.0
127.80	284.0
129.90	326.0
130.90	247.0
134.70	114.0
136.80	230.0
140.80	875.0
141.80	106.0
142.90	1192.0
144.90	452.0
145.80	205.0
147.70	266.0
149.80	106.0
154.80	233.0
156.80	129.0
158.90	120.0
171.80	826.0
173.90	77296.0
174.90	5815.0
175.90	76008.0
176.90	4961.0
178.10	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070