

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111121\
 Data File : VU045733.D
 Acq On : 11 Nov 2021 13:08
 Operator : SY/MD
 Sample : M4608-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 SY-6-20211109

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260

Signal : TIC: VU045733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.755	430	440	450	rBV2	6257	11012	1.46%	0.270%
2	4.629	1007	1023	1040	rBV	3158	8663	1.15%	0.213%
3	5.292	1213	1229	1242	rBV2	118072	247992	32.78%	6.083%
4	5.375	1242	1255	1275	rVB	182156	372677	49.26%	9.142%
5	5.703	1343	1357	1377	rBV	129859	261457	34.56%	6.414%
6	6.253	1513	1528	1543	rBV	283058	525937	69.52%	12.901%
7	7.902	2027	2041	2075	rBV	435857	756488	100.00%	18.557%
8	8.475	2207	2219	2231	rBV2	5274	9224	1.22%	0.226%
9	9.420	2500	2513	2537	rBV	416000	680639	89.97%	16.696%
10	10.635	2879	2891	2911	rBV	322016	509579	67.36%	12.500%
11	10.896	2963	2972	2985	rBV4	5368	9808	1.30%	0.241%
12	11.815	3244	3258	3279	rVB	432073	683181	90.31%	16.758%




Sum of corrected areas: 4076657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111121\
Data File : VU045733.D
Acq On : 11 Nov 2021 13:08
Operator : SY/MD
Sample : M4608-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
SY-6-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

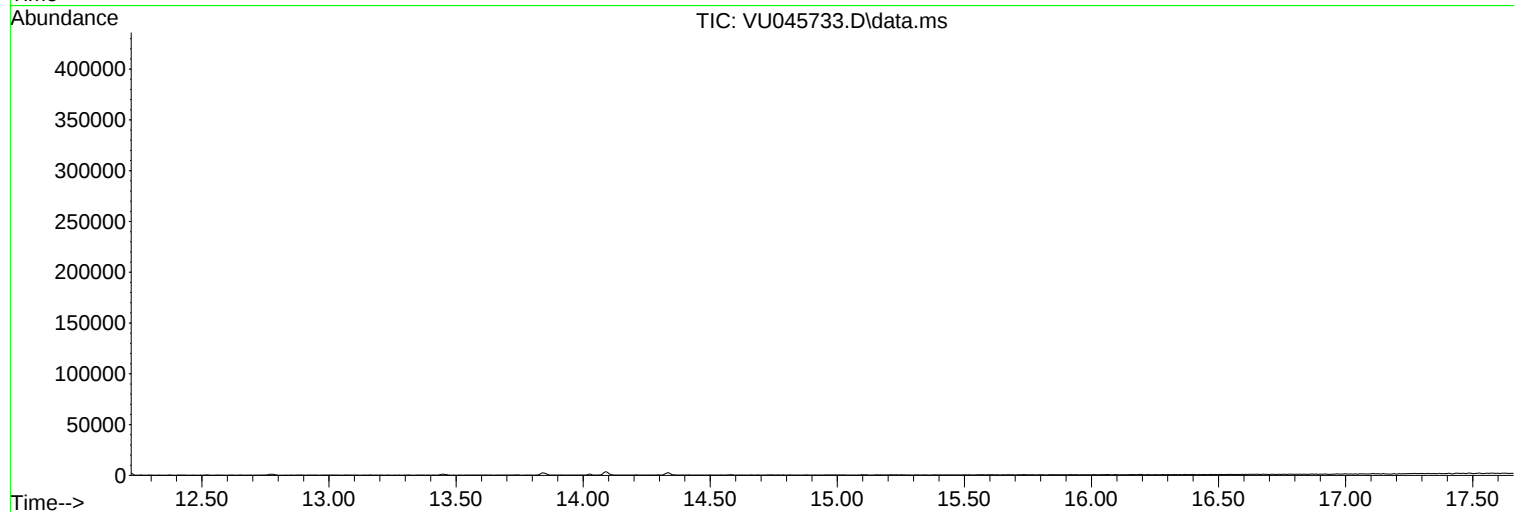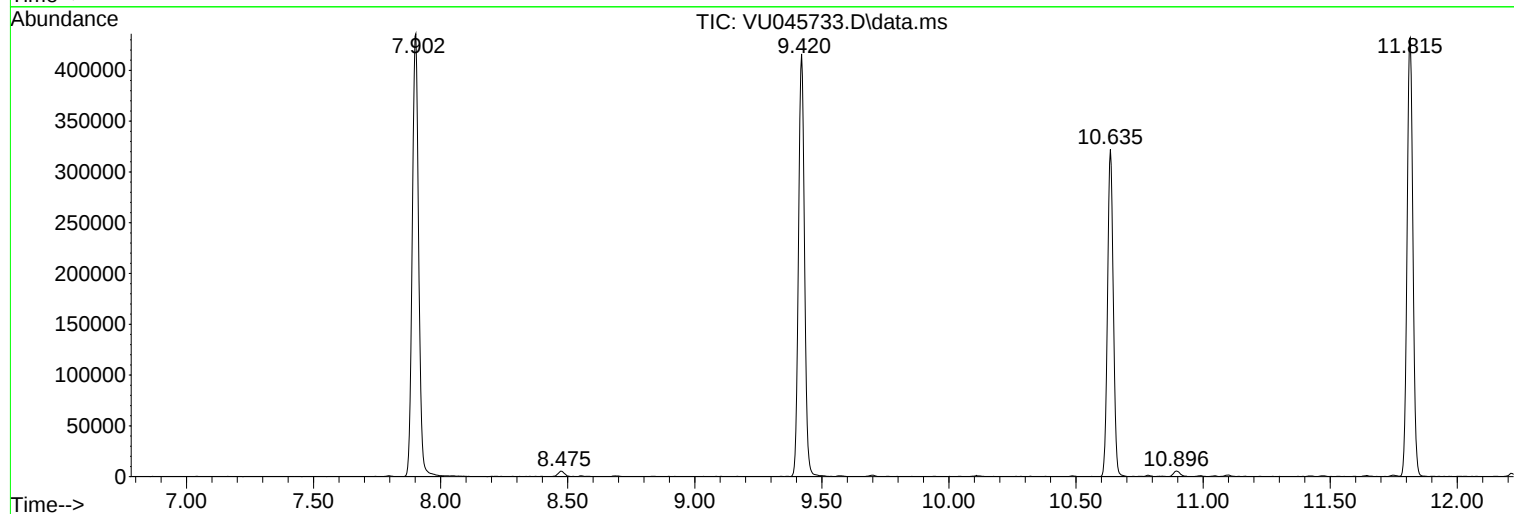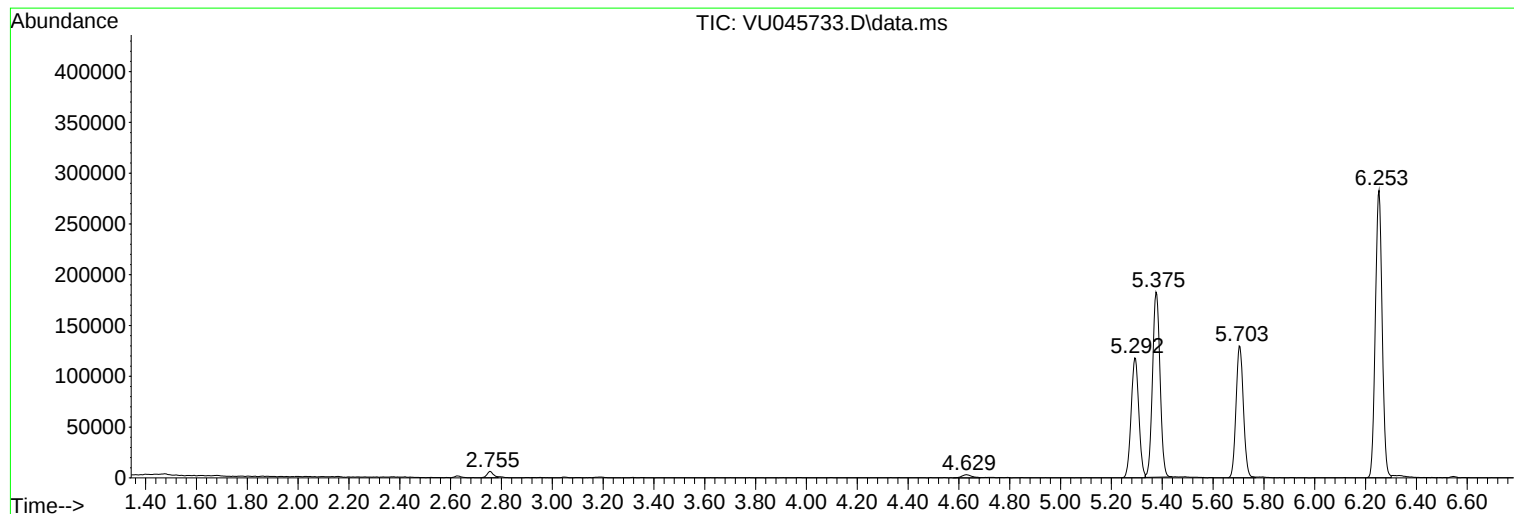

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111121\
Data File : VU045733.D
Acq On : 11 Nov 2021 13:08
Operator : SY/MD
Sample : M4608-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
SY-6-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111121\
Data File : VU045733.D
Acq On : 11 Nov 2021 13:08
Operator : SY/MD
Sample : M4608-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
SY-6-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc