


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111121\
Data File : VU045727.D
Acq On : 11 Nov 2021 09:52
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Title : SW846 8260
Last Update : Fri Nov 05 13:35:16 2021

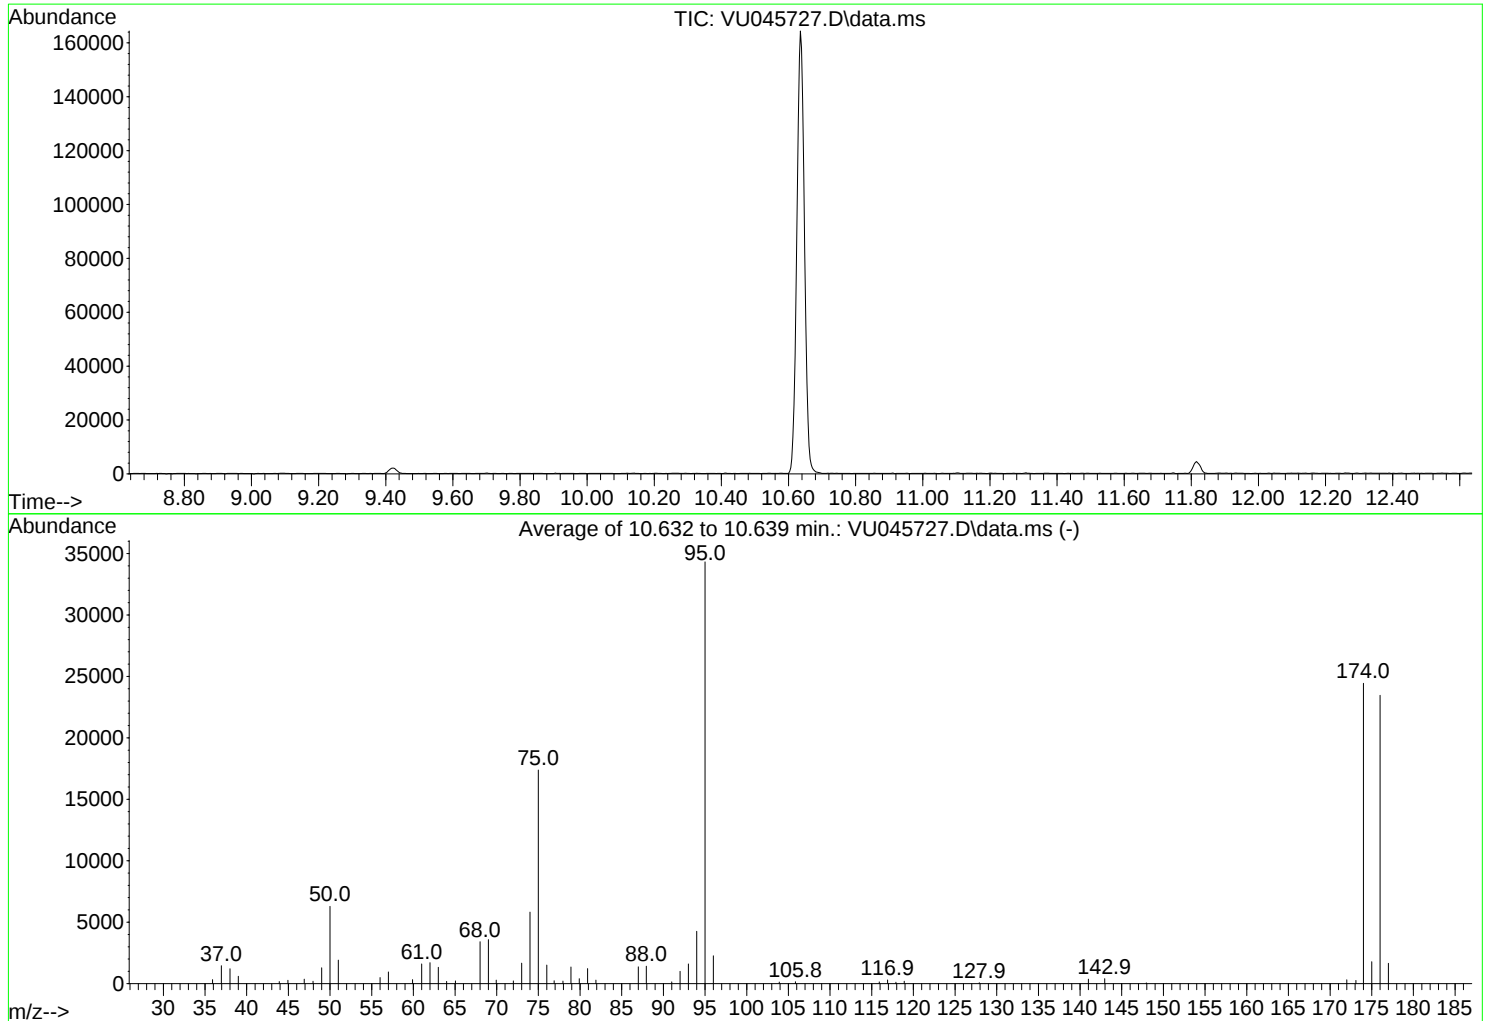

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	6290	PASS
75	95	30	60	50.7	17387	PASS
95	95	100	100	100.0	34325	PASS
96	95	5	9	6.6	2260	PASS
173	174	0.00	2	1.1	259	PASS
174	95	50	100	71.2	24443	PASS
175	174	5	9	7.3	1782	PASS
176	174	95	101	96.0	23467	PASS
177	176	5	9	7.1	1657	PASS