
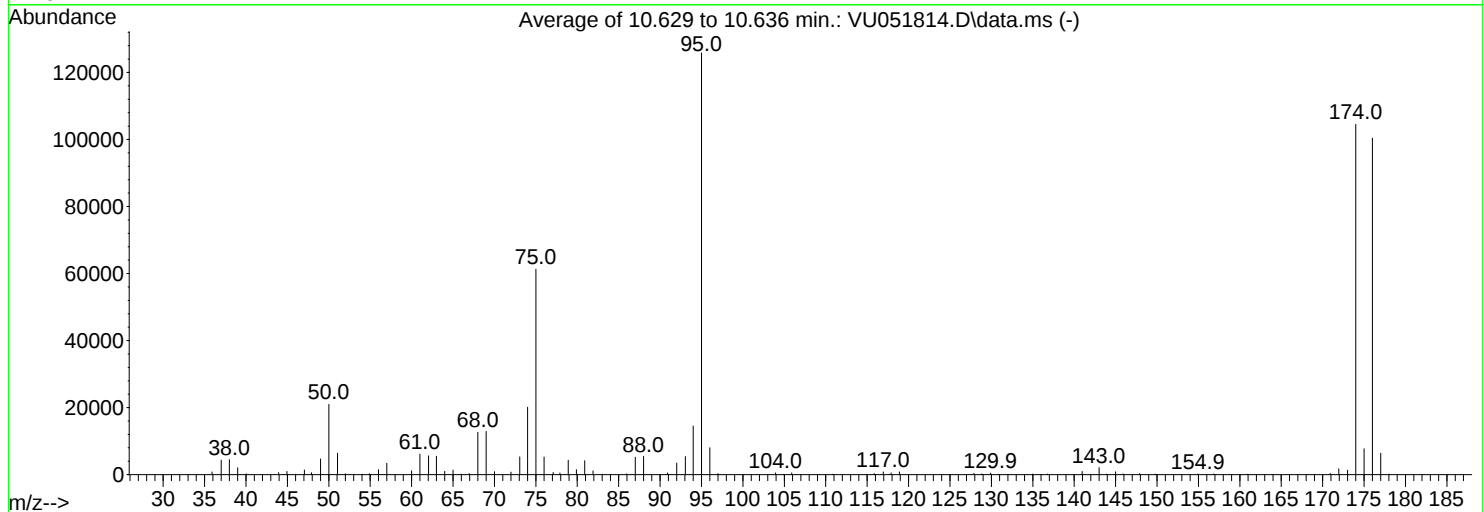


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111122\
 Data File : VU051814.D
 Acq On : 11 Nov 2022 08:56
 Operator : JC/MD
 Sample : BFB168
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB168

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 15 03:00:15 2022

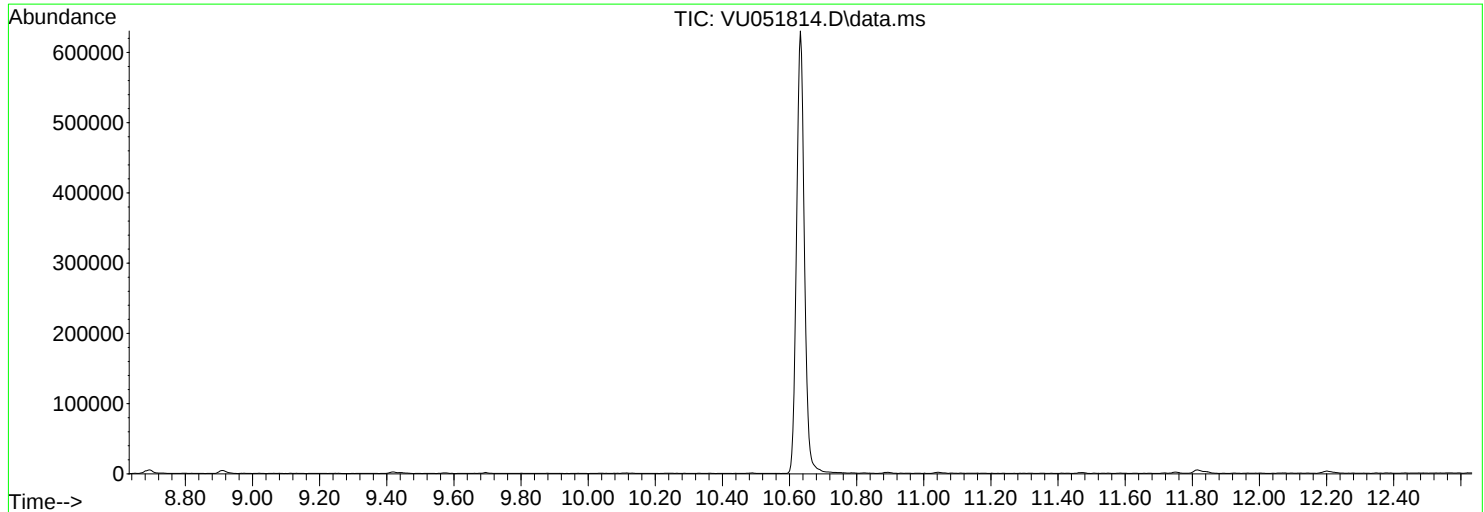

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	20960	PASS
75	95	30	80	48.7	61325	PASS
95	95	100	100	100.0	125853	PASS
96	95	5	9	6.4	8040	PASS
173	174	0.00	2	1.3	1354	PASS
174	95	50	120	83.1	104563	PASS
175	174	5	9	7.4	7717	PASS
176	174	95	101	96.0	100384	PASS
177	176	5	9	6.4	6404	PASS

Scan 2875 (10.584 min): VU051814.D\data.ms
BFB168

m/z	Abundance
39.80	126.0
43.90	499.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	871.0
37.00	4353.0
38.00	4628.0
39.00	1912.0
40.00	275.0
43.00	108.0
44.00	1282.0
44.90	1110.0
46.00	175.0
47.00	1373.0
47.90	579.0
49.00	4533.0
50.00	21040.0
51.00	6583.0
52.00	278.0
53.00	144.0
54.10	151.0
54.80	284.0
56.00	1400.0
57.00	3358.0
58.00	112.0
60.00	1172.0
61.00	6273.0
62.00	5946.0
63.00	5511.0
64.00	978.0
65.00	1260.0
66.00	204.0
66.90	338.0
68.00	12526.0
69.00	12712.0
70.00	862.0
72.00	721.0
73.00	5091.0
74.00	20192.0
75.00	61640.0
76.00	5277.0
77.10	733.0
77.90	496.0
78.90	4342.0
79.90	1420.0
80.90	4221.0
81.90	1077.0
83.00	151.0
86.00	178.0
87.00	5208.0
88.00	5352.0
90.90	587.0
92.00	3529.0
93.00	5142.0
94.00	14076.0
95.00	125720.0
96.00	8298.0
97.00	349.0
103.90	498.0
104.90	123.0
105.90	523.0
110.80	166.0
114.90	156.0
115.80	328.0
117.00	835.0
117.90	492.0
118.90	778.0
127.90	419.0
128.80	220.0
129.90	538.0
130.90	179.0
135.00	184.0
136.80	160.0
141.00	876.0
141.90	145.0
143.00	2060.0
143.90	195.0
145.00	922.0
145.90	257.0
147.90	300.0
149.80	117.0
155.00	255.0
156.90	234.0
158.80	105.0
160.90	162.0
170.90	354.0
172.00	1774.0
173.00	1305.0
174.00	101032.0
175.00	7729.0
176.00	96480.0
177.00	6301.0
178.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	843.0
37.00	4549.0
38.00	4611.0
39.00	2132.0
40.00	274.0
43.00	115.0
44.00	1150.0
45.00	967.0
46.00	160.0
47.10	1401.0
47.90	616.0
49.00	4914.0
50.00	21624.0
51.10	6524.0
52.00	277.0
53.10	141.0
54.10	155.0
54.90	317.0
56.00	1566.0
57.00	3469.0
58.00	109.0
60.00	1195.0
61.00	6321.0
62.00	5836.0
63.00	5692.0
64.00	1057.0
65.00	1446.0
66.00	183.0
66.90	385.0
68.00	13095.0
69.00	13473.0
70.00	977.0
72.00	816.0
73.00	5469.0
74.00	20728.0
75.00	63128.0
76.00	5463.0
77.10	651.0
77.90	556.0
78.90	4438.0
79.90	1521.0
80.90	4224.0
81.90	1208.0
83.00	141.0
86.00	249.0
87.00	5379.0
88.00	5493.0
90.90	537.0
92.00	3564.0
93.00	5662.0
94.00	15104.0
95.00	129912.0
96.00	8313.0
97.00	353.0
104.00	558.0
104.90	127.0
105.90	531.0
110.80	154.0
115.00	161.0
115.90	373.0
116.90	875.0
117.90	520.0
118.90	846.0
127.90	440.0
128.80	222.0
129.90	483.0
130.90	181.0
135.00	229.0
136.80	216.0
140.90	960.0
142.00	160.0
143.00	2178.0
143.90	231.0
145.00	926.0
145.90	255.0
147.90	350.0
149.90	138.0
155.00	267.0
156.80	255.0
160.90	176.0
170.90	359.0
172.00	1780.0
173.00	1426.0
174.00	107736.0
175.00	7966.0
176.00	104072.0
177.00	6707.0
178.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168

m/z	Abundance
35.90	738.0
37.00	4140.0
38.00	4292.0
39.00	2152.0
40.10	258.0
42.90	122.0
44.00	1000.0
45.00	798.0
46.00	109.0
47.00	1350.0
47.90	583.0
49.00	4650.0
50.00	20216.0
51.10	6111.0
52.00	313.0
53.10	158.0
54.10	114.0
55.00	317.0
56.00	1560.0
57.00	3295.0
58.00	140.0
60.00	1078.0
61.00	5785.0
62.10	5192.0
63.00	5246.0
64.00	1003.0
65.00	1466.0
66.00	162.0
67.00	326.0
68.00	12381.0
69.00	12434.0
70.00	950.0
72.00	808.0
73.10	5326.0
74.00	19328.0
75.00	59208.0
76.00	4959.0
77.10	563.0
77.90	560.0
78.90	4077.0
79.90	1470.0
80.90	4025.0
81.90	1149.0
83.10	111.0
85.90	274.0
87.00	5073.0
88.00	5462.0
90.90	393.0
92.00	3190.0
93.10	5428.0
94.00	14436.0
95.00	121928.0
96.00	7510.0
97.00	293.0
104.00	540.0
104.90	122.0
105.90	537.0
107.00	126.0
110.90	109.0
115.00	145.0
115.90	345.0
116.90	789.0
117.90	502.0
118.90	848.0
127.90	392.0
128.90	251.0
129.90	381.0
130.90	152.0
134.90	253.0
136.80	260.0
140.90	1009.0
142.00	132.0
143.00	2009.0
143.90	162.0
145.00	726.0
145.90	242.0
147.90	321.0
149.90	145.0
154.90	244.0
156.80	226.0
160.90	152.0
170.90	370.0
171.90	1723.0
173.00	1330.0
174.00	104920.0
175.00	7456.0
176.00	100600.0
177.00	6204.0
178.00	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB168