
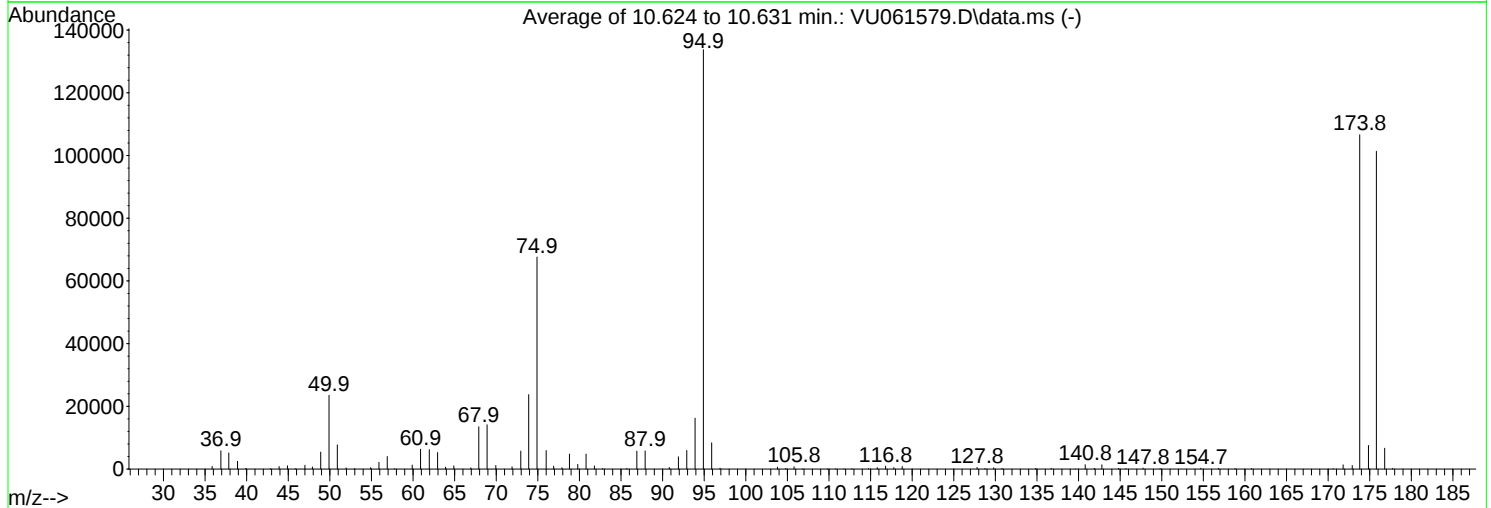


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111124\
Data File : VU061579.D
Acq On : 11 Nov 2024 09:00
Operator : MD/SY
Sample : BFB024
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB024

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 12 03:43:56 2024

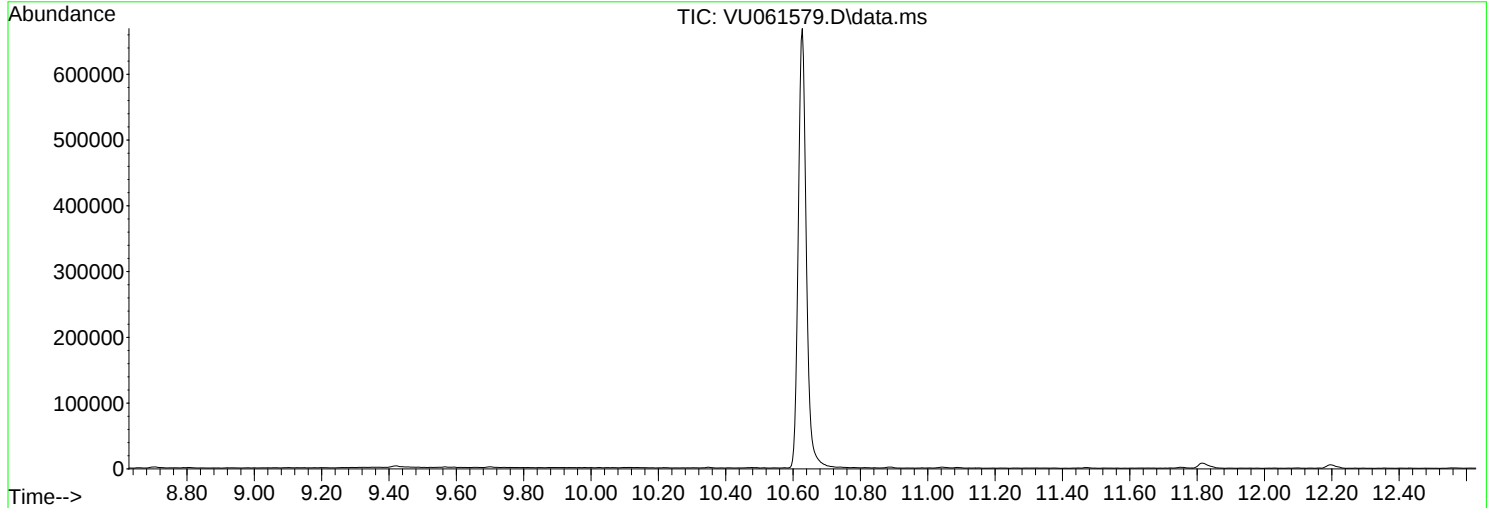

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	23515	PASS
75	95	30	80	50.6	67613	PASS
95	95	100	100	100.0	133736	PASS
96	95	5	9	6.3	8392	PASS
173	174	0.00	2	1.1	1155	PASS
174	95	50	120	79.7	106629	PASS
175	174	5	9	7.1	7535	PASS
176	174	95	101	95.1	101355	PASS
177	176	5	9	6.6	6650	PASS

m/z	Abundance
35.90	975.0
37.80	295.0
43.90	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	1958.0
36.90	5959.0
37.90	5611.0
38.90	2567.0
39.90	240.0
42.90	110.0
43.90	1101.0
44.90	1059.0
45.90	161.0
47.00	1303.0
47.90	762.0
48.90	5336.0
49.90	24344.0
50.90	7898.0
52.00	320.0
52.90	145.0
54.90	487.0
55.90	2181.0
56.90	3941.0
57.80	131.0
59.90	1294.0
60.90	6490.0
62.00	6352.0
62.90	5375.0
63.90	642.0
64.90	1082.0
67.00	407.0
67.90	14145.0
68.90	14578.0
69.90	1196.0
71.90	756.0
72.90	5954.0
73.90	24232.0
74.90	68104.0
76.00	6134.0
76.90	985.0
77.90	386.0
78.80	4903.0
79.80	1417.0
80.80	4854.0
81.80	1037.0
82.80	203.0
85.70	241.0
86.90	5809.0
87.90	5594.0
90.80	487.0
91.90	3793.0
92.90	6053.0
93.90	16211.0
94.90	133824.0
95.90	8680.0
96.90	279.0
103.80	619.0
104.80	243.0
105.80	731.0
110.80	137.0
112.70	100.0
114.80	147.0
115.80	470.0
116.80	927.0
117.80	478.0
118.80	806.0
127.80	581.0
128.70	168.0
129.80	458.0
130.80	256.0
134.90	219.0
136.70	259.0
140.80	1365.0
141.90	196.0
142.80	1444.0
144.80	191.0
145.70	162.0
147.80	315.0
149.80	134.0
154.70	302.0
156.80	255.0
158.80	149.0
160.80	170.0
170.60	112.0
171.80	1339.0
172.90	1013.0
173.80	105448.0
174.90	7550.0
175.80	100096.0
176.80	6624.0
177.70	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	1850.0
36.90	6025.0
37.90	5601.0
38.90	2568.0
39.90	207.0
42.80	108.0
43.90	1114.0
44.90	1099.0
45.90	128.0
47.00	1292.0
47.90	708.0
48.90	5616.0
49.90	24272.0
50.90	7914.0
51.90	392.0
52.90	151.0
54.90	446.0
55.90	2215.0
56.90	4171.0
57.80	112.0
59.90	1286.0
60.90	6551.0
61.90	6331.0
63.00	5440.0
63.90	644.0
64.90	1074.0
66.90	410.0
67.90	13754.0
68.90	14584.0
70.00	1135.0
71.90	758.0
72.90	5943.0
73.90	24480.0
74.90	69736.0
76.00	6034.0
76.90	946.0
77.90	449.0
78.80	4944.0
79.80	1550.0
80.80	4959.0
81.80	1015.0
82.80	197.0
85.70	221.0
86.90	5962.0
87.90	6093.0
90.80	551.0
91.90	3997.0
92.90	6067.0
93.90	16840.0
94.90	138240.0
95.90	8626.0
96.90	291.0
103.80	656.0
104.80	220.0
105.80	806.0
106.80	110.0
109.80	103.0
110.80	102.0
112.70	105.0
114.70	146.0
115.80	501.0
116.80	922.0
117.80	493.0
118.80	878.0
127.80	558.0
128.80	201.0
129.80	446.0
130.80	237.0
134.90	238.0
136.70	237.0
140.80	1432.0
141.90	217.0
142.80	1404.0
144.80	218.0
145.70	176.0
147.70	346.0
149.80	116.0
154.70	292.0
156.80	244.0
158.80	208.0
160.80	175.0
170.60	109.0
171.80	1436.0
172.90	1184.0
173.80	110152.0
174.80	7774.0
175.80	104800.0
176.80	6870.0
177.80	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	1648.0
36.90	5540.0
37.90	5124.0
38.90	2301.0
39.90	176.0
42.80	107.0
43.90	1012.0
44.90	1047.0
45.80	115.0
47.00	1115.0
47.90	619.0
48.90	5320.0
49.90	21928.0
50.90	7346.0
51.90	400.0
53.00	150.0
54.90	403.0
55.90	2013.0
56.90	3940.0
57.80	102.0
59.90	1266.0
60.90	5969.0
61.90	5960.0
62.90	4978.0
63.90	609.0
64.90	948.0
66.90	393.0
67.90	12551.0
68.90	13261.0
69.90	1063.0
71.90	699.0
73.00	5317.0
73.90	22520.0
74.90	65000.0
76.00	5570.0
76.90	822.0
77.90	468.0
78.80	4594.0
79.80	1512.0
80.80	4528.0
81.80	948.0
82.80	165.0
85.70	202.0
86.90	5382.0
87.90	5754.0
90.80	567.0
91.90	3936.0
92.90	5687.0
93.90	15703.0
94.90	129144.0
95.90	7871.0
96.90	256.0
103.80	657.0
104.80	198.0
105.80	742.0
106.90	134.0
109.80	100.0
111.80	100.0
112.80	114.0
114.70	130.0
115.80	481.0
116.80	886.0
117.80	486.0
118.80	808.0
127.80	483.0
128.80	231.0
129.80	383.0
130.80	195.0
134.80	232.0
136.70	220.0
139.60	110.0
140.80	1430.0
141.90	190.0
142.80	1278.0
144.80	230.0
145.70	151.0
147.70	339.0
149.80	103.0
154.70	307.0
156.80	210.0
158.80	191.0
160.80	132.0
170.60	103.0
171.80	1330.0
172.90	1267.0
173.80	104288.0
174.80	7281.0
175.80	99168.0
176.80	6457.0
177.80	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024