


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111125\
Data File : VU063697.D
Acq On : 11 Nov 2025 08:38
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U111025W.M
Title : SW846 8260
Last Update : Tue Nov 11 01:41:19 2025

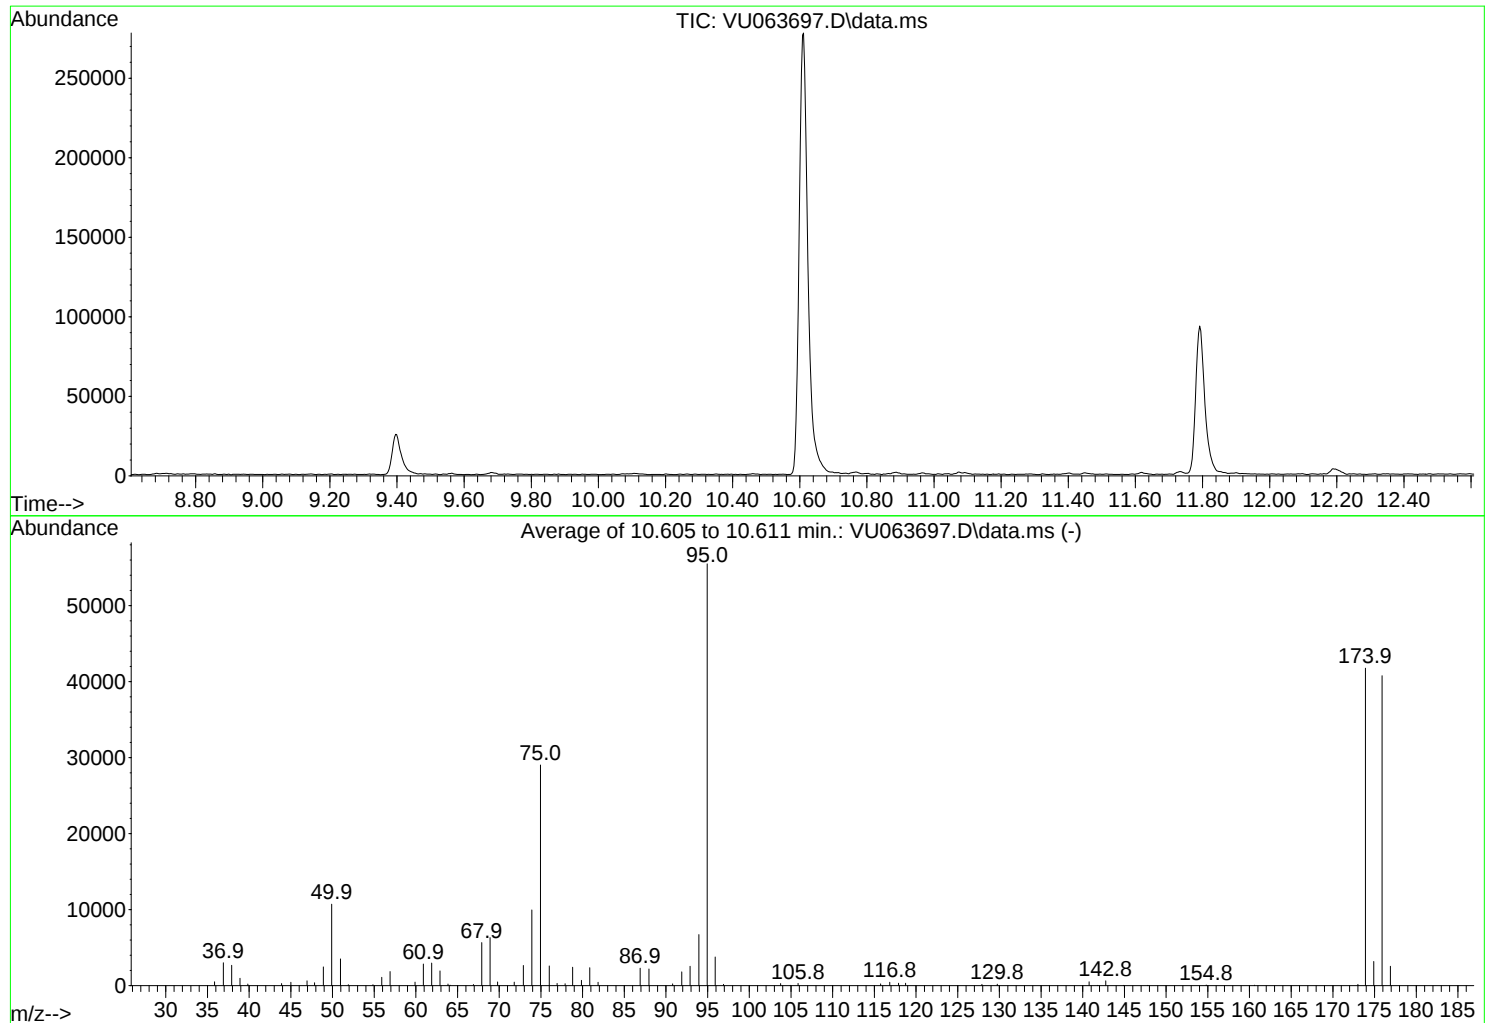

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10708	PASS
75	95	30	60	52.3	29029	PASS
95	95	100	100	100.0	55499	PASS
96	95	5	9	6.8	3770	PASS
173	174	0.00	2	0.4	164	PASS
174	95	50	100	75.3	41773	PASS
175	174	5	9	7.6	3180	PASS
176	174	95	101	97.6	40784	PASS
177	176	5	9	6.2	2539	PASS