


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU111218\
Data File : VU028054.D
Acq On : 12 Nov 2018 09:18
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Title : SW846 8260
Last Update : Fri Nov 02 02:28:20 2018

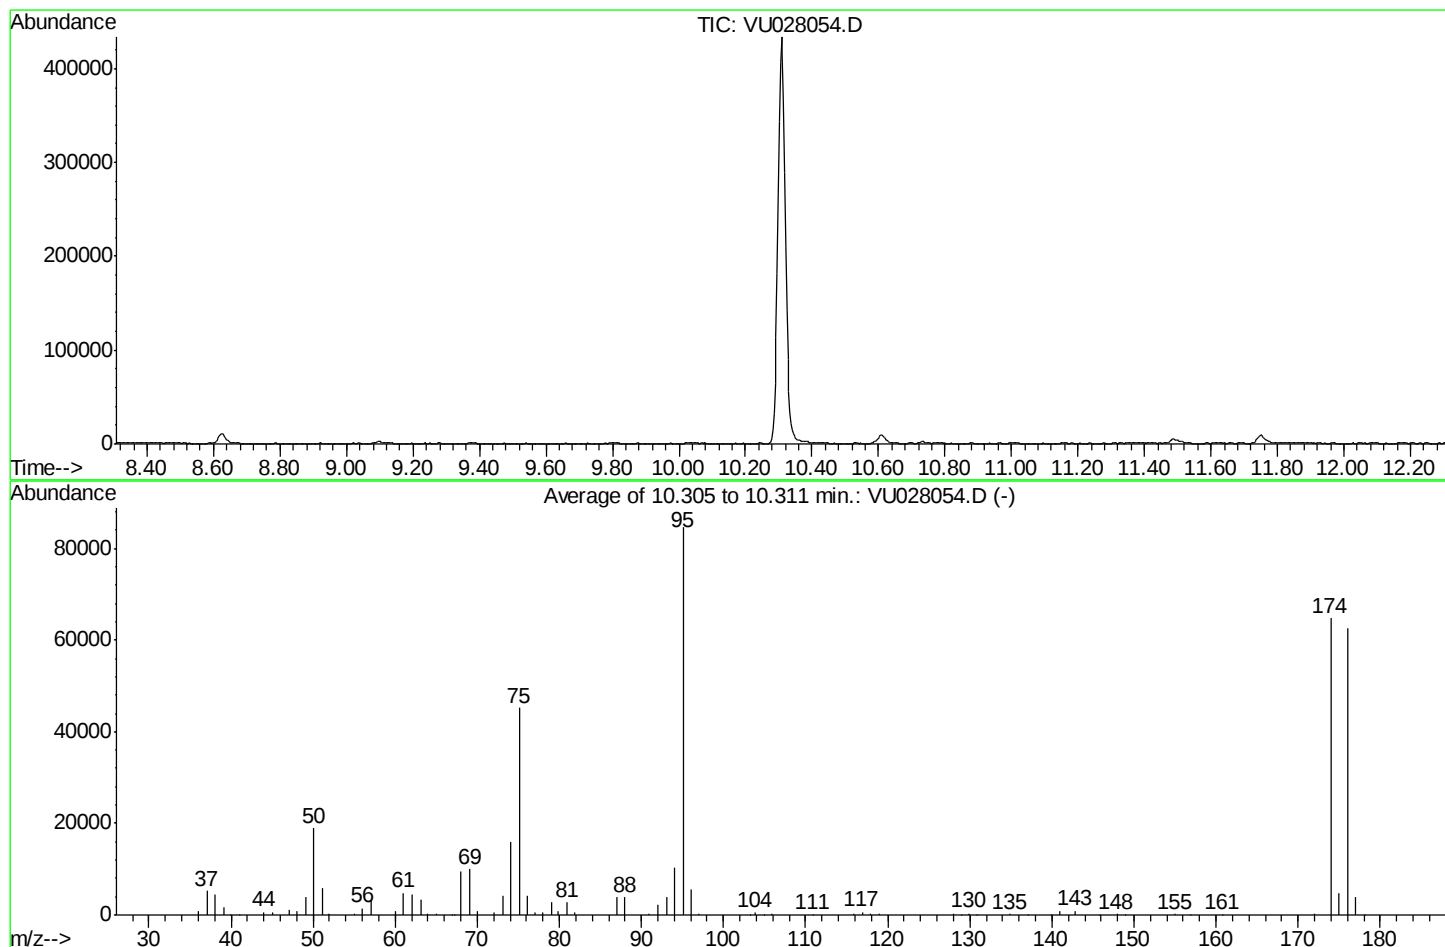

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	18981	PASS
75	95	30	60	53.4	45197	PASS
95	95	100	100	100.0	84613	PASS
96	95	5	9	6.7	5651	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.6	64781	PASS
175	174	5	9	7.4	4791	PASS
176	174	95	101	96.8	62682	PASS
177	176	5	9	6.1	3834	PASS