


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111219\
Data File : VU035693.D
Acq On : 12 Nov 2019 14:21
Operator : JC/SP
Sample : K5798-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFLW5

Manual Integrations
APPROVED

MMDadoda
11/13/2019 11:21:04 AM

Quant Time: Nov 13 01:21:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 00:43:14 2019
Response via : Initial Calibration

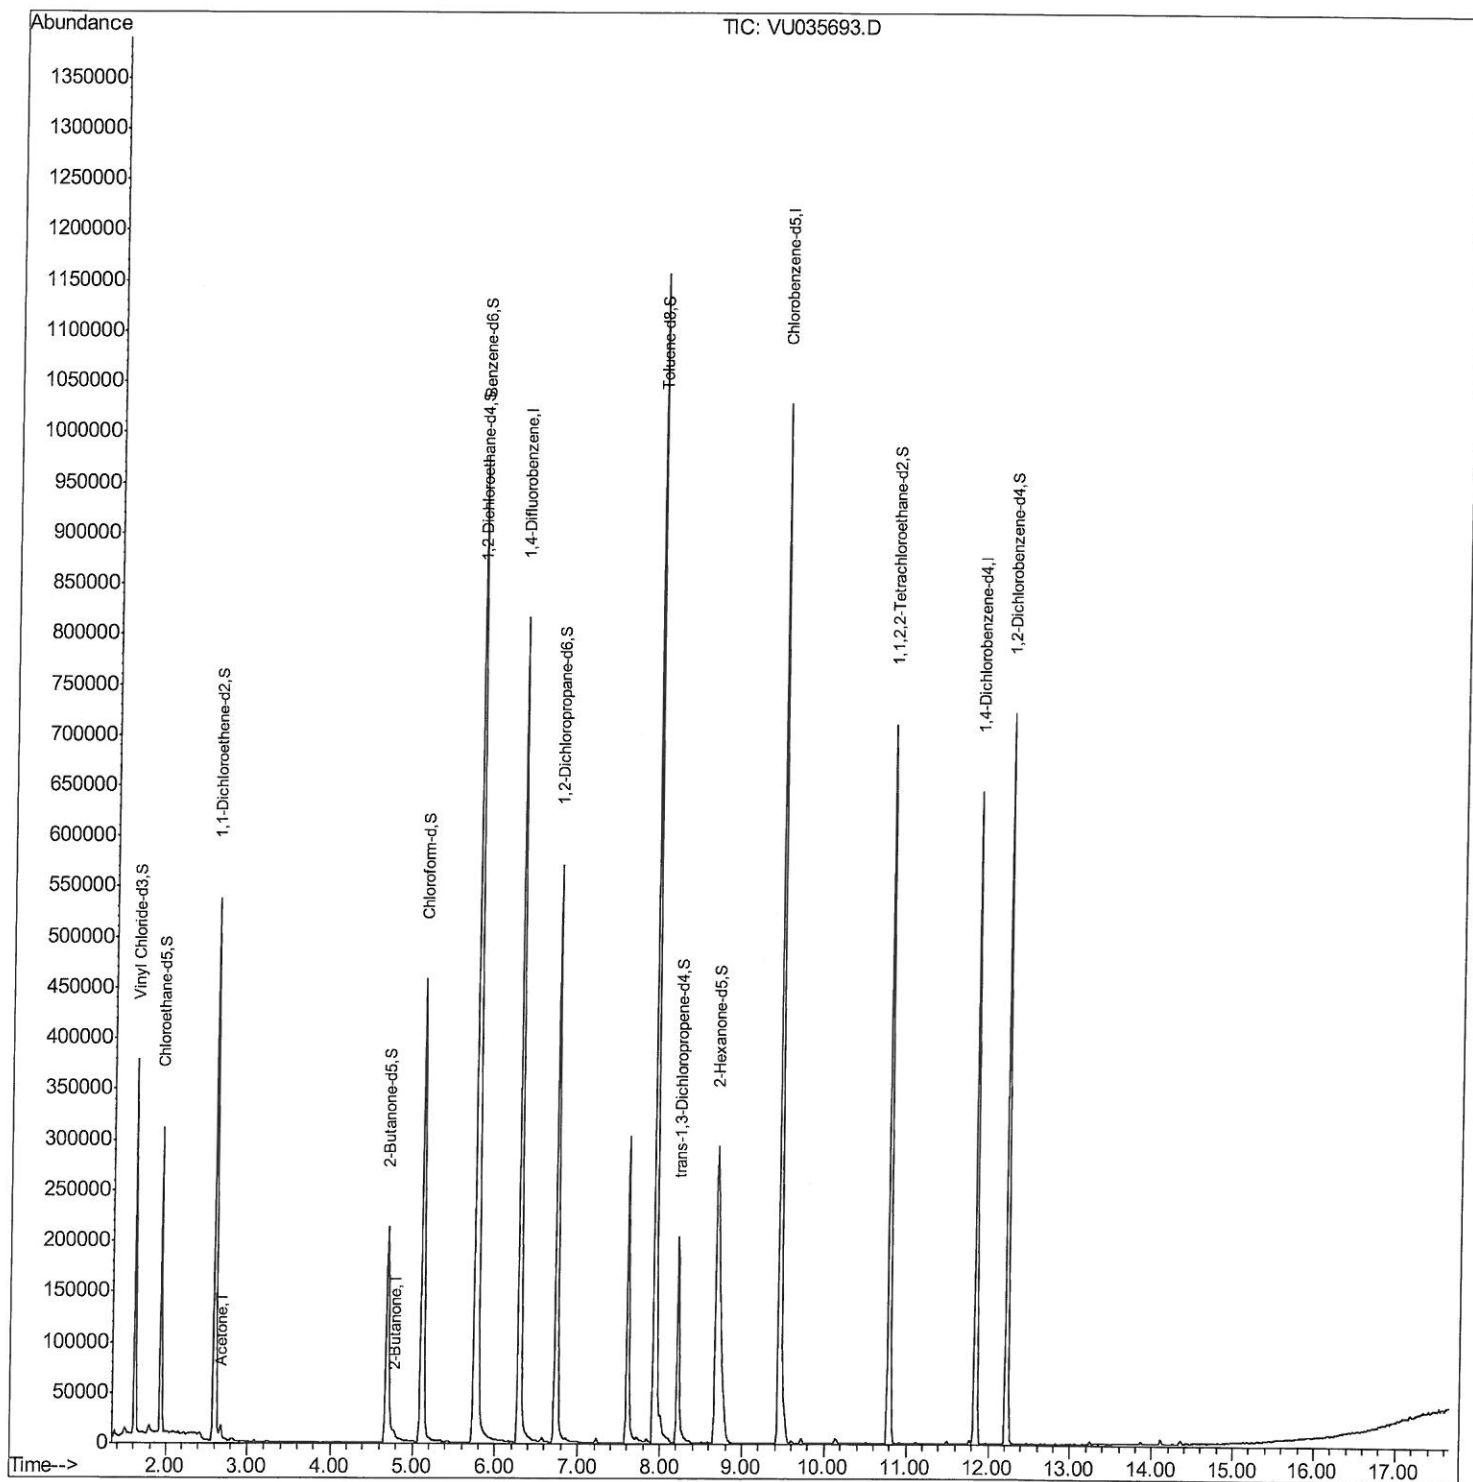

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111219\
Data File : VU035693.D
Acq On : 12 Nov 2019 14:21
Operator : JC/SP
Sample : K5798-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFLW5

Manual Integrations
APPROVED

MMDadoda
11/13/2019 11:21:04 AM

Quant Time: Nov 13 01:19:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 00:43:14 2019
Response via : Initial Calibration

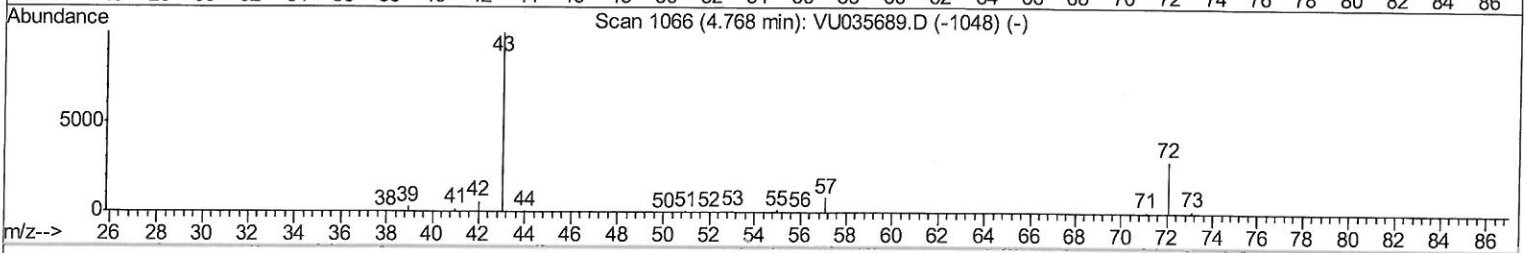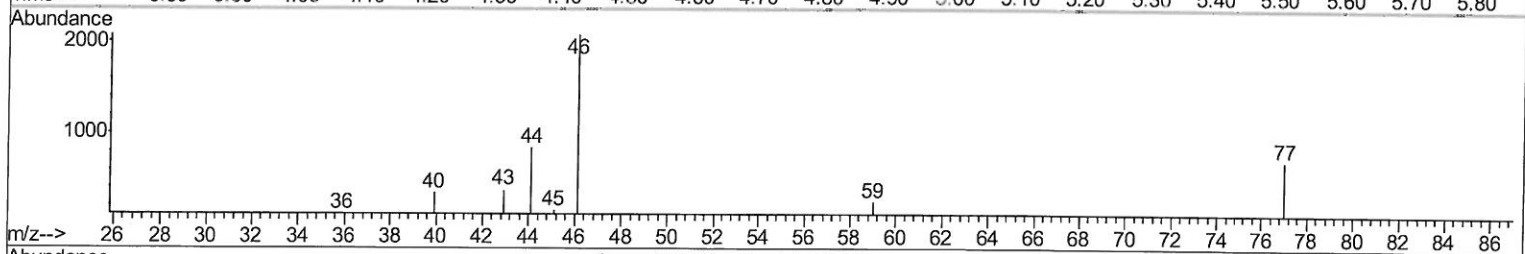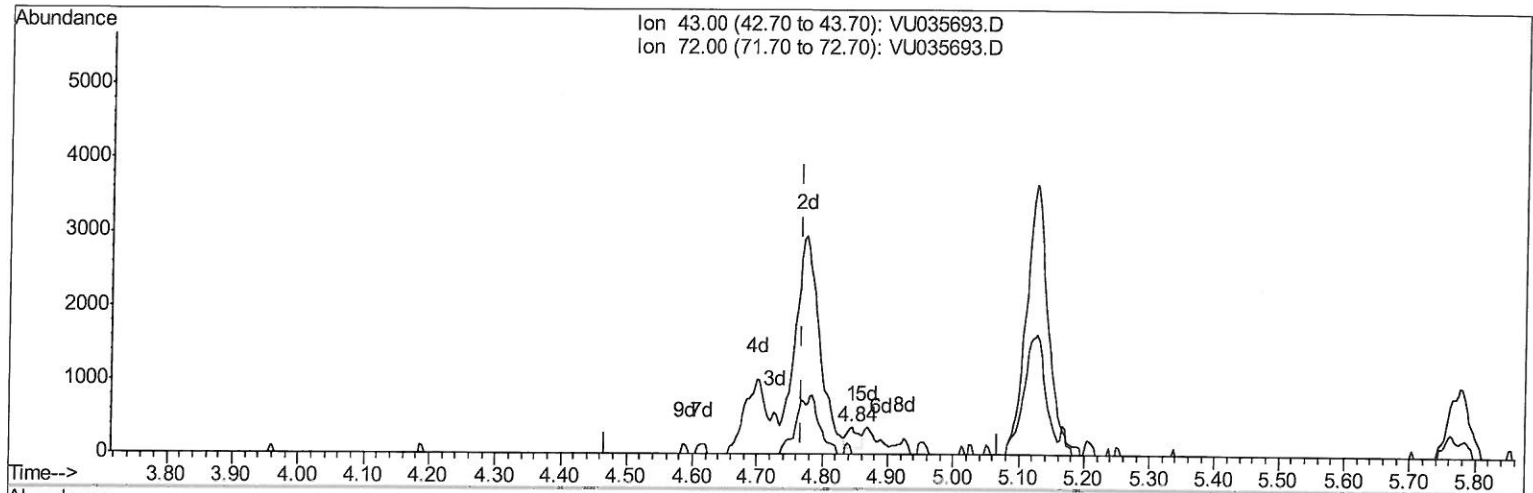

TIC: VU035693.D

(22) 2-Butanone (T)

4.845min (+0.077) 0.10ug/L

response 373

Ion	Exp%	Act%
43.00	100	100
72.00	26.90	19.57
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111219\
 Data File : VU035693.D
 Acq On : 12 Nov 2019 14:21
 Operator : JC/SP
 Sample : K5798-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 BFLW5

Manual Integrations
 APPROVED

MMDadoda
 11/13/2019 11:21:04 AM

Ouant Time: Nov 13 01:19:31 2019
 Ouant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 00:43:14 2019
 Response via : Initial Calibration

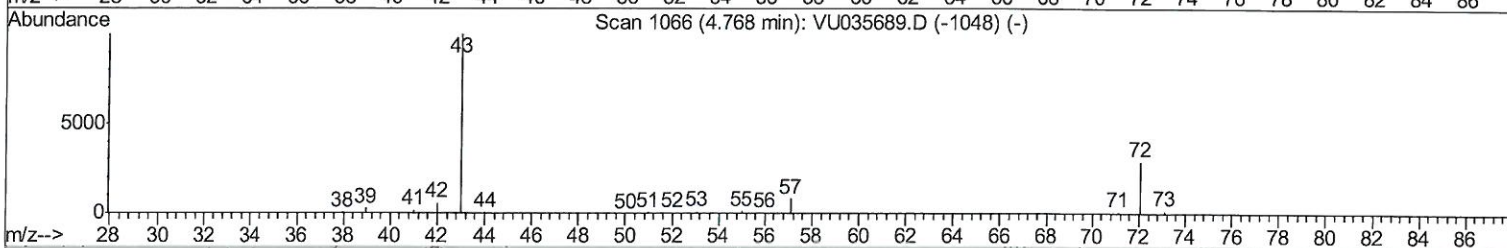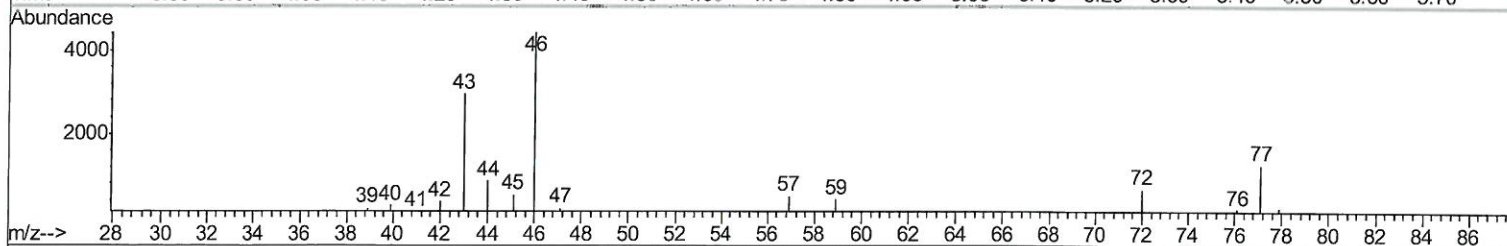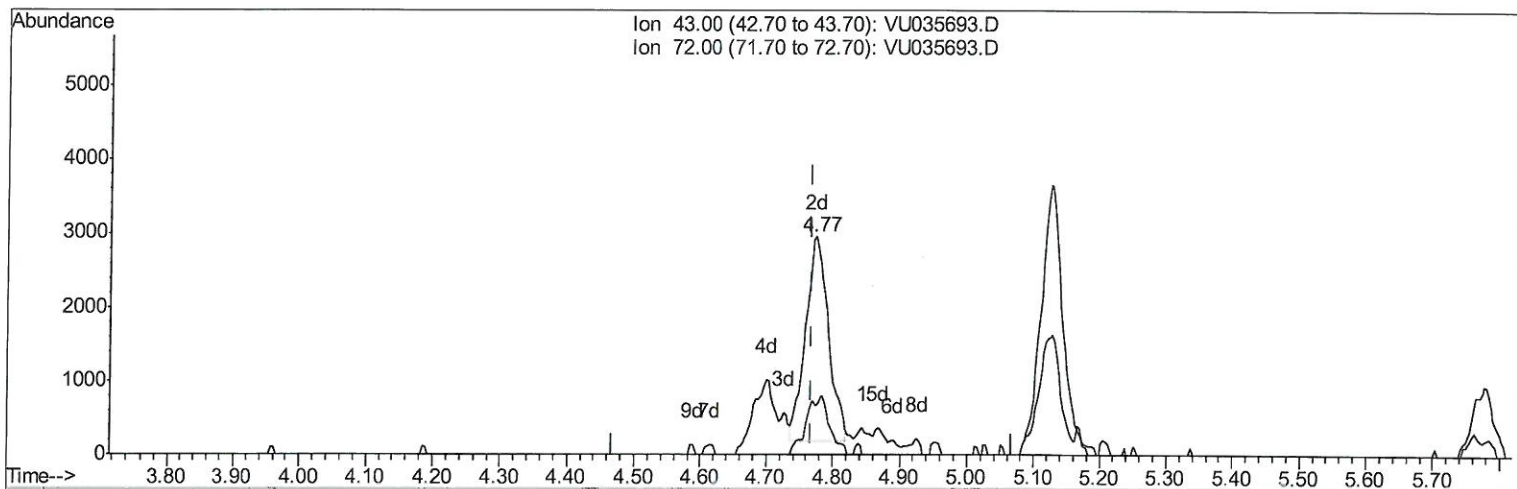

TIC: VU035693.D

(22) 2-Butanone (T)

4.774min (+0.006) 1.71ug/L m

response 6677

Ion	Exp%	Act%
43.00	100	100
72.00	26.90	1.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111219\
 Data File : VU035693.D
 Acq On : 12 Nov 2019 14:21
 Operator : JC/SP
 Sample : K5798-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 BFLW5

Manual Integrations
 APPROVED

MMDadoda
 11/13/2019 11:21:04 AM

Quant Time: Nov 13 01:21:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 00:43:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	712226	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	682162	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	198960	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	257584	44.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.56%
7) Chloroethane-d5	1.93	69	224544	48.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.76%
11) 1,1-Dichloroethene-d2	2.60	63	320267	35.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.60%
21) 2-Butanone-d5	4.69	46	331749	98.73	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.73%
24) Chloroform-d	5.11	84	428558	48.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.48%
26) 1,2-Dichloroethane-d4	5.75	65	270932	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.56%
32) Benzene-d6	5.77	84	923708	51.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.90%
36) 1,2-Dichloropropane-d6	6.73	67	293274	50.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.72%
41) Toluene-d8	7.93	98	835891	49.84	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.68%
43) trans-1,3-Dichloropropene-	8.21	79	135031	50.84	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.68%
47) 2-Hexanone-d5	8.68	63	212634	96.21	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.21%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	390670	47.64	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.28%
64) 1,2-Dichlorobenzene-d4	12.22	152	215450	53.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.38%

Target Compounds

					Ovalue	
13) Acetone	2.67	43	15336	5.188	ug/L	96
22) 2-Butanone	4.77	43	6677m	1.711	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 m2
 11/21/19