


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111219\
 Data File : VU035688.D
 Acq On : 12 Nov 2019 09:30
 Operator : JC/SP
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 13 15:38:57 2019

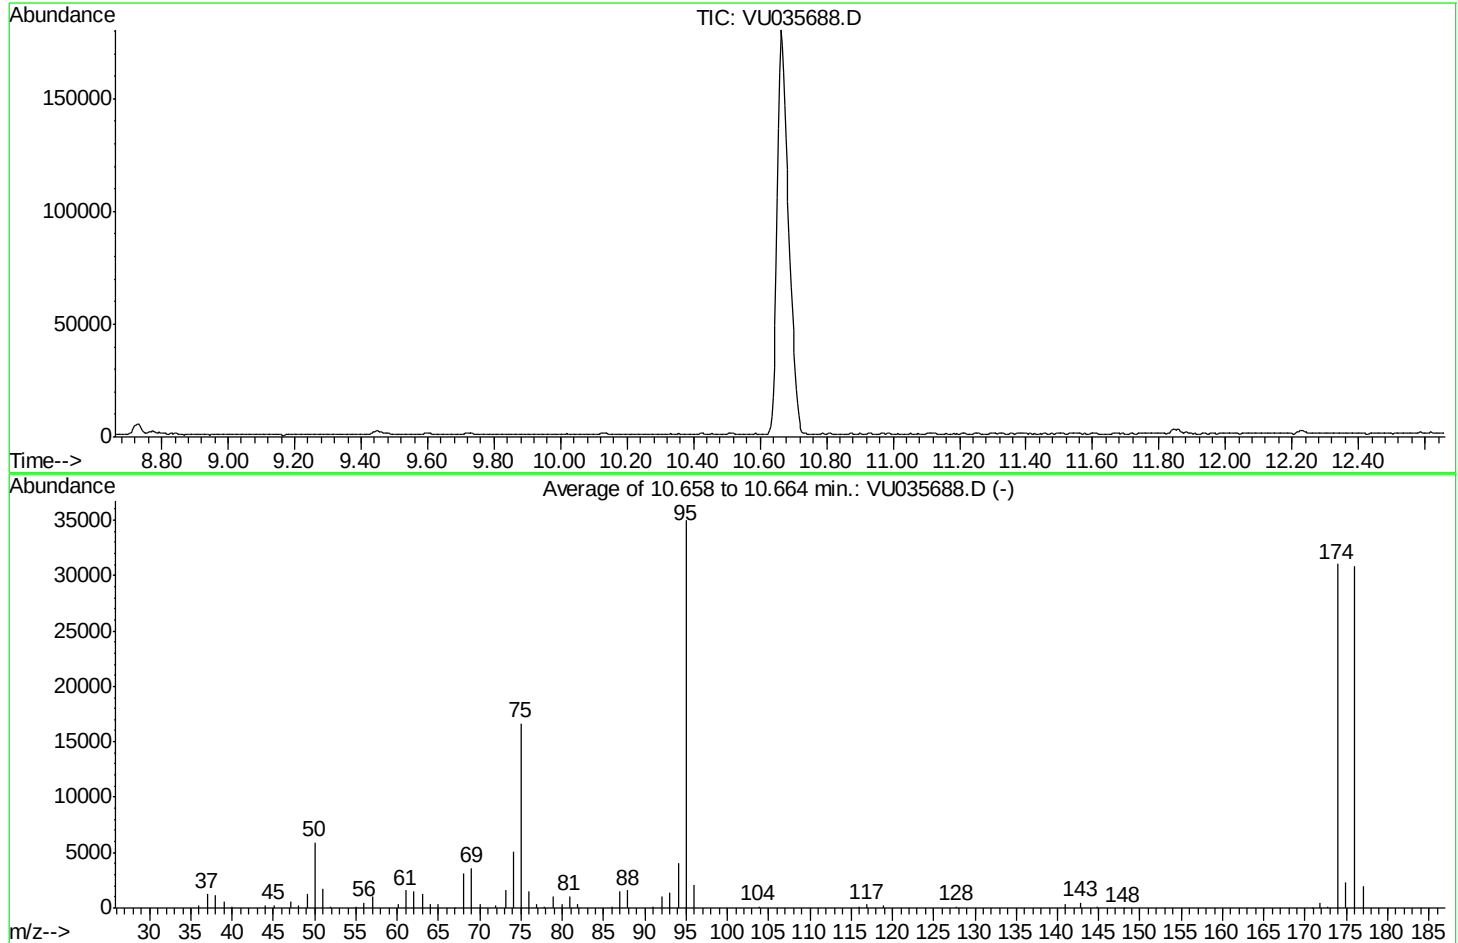

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	5912	PASS
75	95	30	80	47.7	16691	PASS
95	95	100	100	100.0	34976	PASS
96	95	5	9	6.0	2113	PASS
173	174	0.00	2	0.4	121	PASS
174	95	50	120	88.8	31058	PASS
175	174	5	9	7.4	2307	PASS
176	174	95	101	99.1	30792	PASS
177	176	5	9	6.3	1953	PASS

m/z	Abundance
35.90	171.0
37.00	1303.0
38.00	1158.0
39.00	563.0
40.00	280.0
44.00	1256.0
45.10	229.0
47.10	553.0
48.00	146.0
49.00	1306.0
50.00	5582.0
51.00	1710.0
55.00	184.0
55.90	375.0
57.00	953.0
60.10	339.0
61.00	1644.0
62.00	1304.0
63.00	1293.0
64.00	283.0
65.00	277.0
68.00	2882.0
69.00	3496.0
70.10	287.0
71.90	184.0
73.10	1533.0
74.10	4747.0
75.00	15265.0
76.00	1469.0
76.80	291.0
77.80	193.0
78.90	1057.0
80.10	317.0
80.90	987.0
81.90	309.0
86.90	1453.0
87.90	1420.0
90.90	176.0
92.00	823.0
93.00	1223.0
94.10	3616.0
95.00	33576.0
96.00	1998.0
103.90	154.0
115.90	165.0
116.90	263.0
118.90	266.0
127.80	136.0
141.00	313.0
142.90	461.0
144.80	125.0
170.90	100.0
171.80	402.0
172.80	365.0
173.90	28440.0
174.90	2077.0
176.00	28208.0
177.00	1845.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.80	209.0
37.00	1315.0
38.00	1196.0
39.00	620.0
40.00	297.0
44.00	1225.0
45.00	244.0
47.10	567.0
48.00	255.0
49.10	1317.0
50.00	6053.0
51.00	1783.0
51.90	118.0
55.00	178.0
56.00	489.0
57.00	1007.0
60.10	363.0
61.00	1603.0
62.00	1591.0
63.00	1309.0
64.00	310.0
65.00	330.0
68.00	3144.0
69.00	3730.0
70.10	326.0
71.90	233.0
73.10	1721.0
74.10	5164.0
75.00	17208.0
76.00	1486.0
76.90	309.0
77.80	174.0
78.90	1064.0
80.00	351.0
80.90	1117.0
81.80	339.0
86.00	101.0
86.90	1483.0
87.90	1677.0
90.90	166.0
92.00	1026.0
93.00	1464.0
94.00	4120.0
95.00	35840.0
96.00	2112.0
103.90	164.0
116.00	169.0
116.90	305.0
118.90	259.0
127.80	141.0
141.00	321.0
142.80	513.0
144.70	186.0
171.80	449.0
173.90	31560.0
174.90	2334.0
176.00	31584.0
177.00	1990.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.80	231.0
37.00	1265.0
38.00	1158.0
39.00	594.0
40.00	280.0
43.90	1251.0
45.00	230.0
47.10	475.0
47.90	318.0
49.00	1245.0
50.00	6102.0
51.00	1815.0
51.90	105.0
55.00	111.0
56.00	565.0
57.00	1025.0
60.10	359.0
61.00	1520.0
62.00	1745.0
63.00	1229.0
63.90	308.0
65.00	382.0
67.00	110.0
68.00	3176.0
69.00	3632.0
70.00	322.0
71.90	245.0
73.10	1768.0
74.10	5382.0
75.00	17600.0
76.00	1445.0
76.90	313.0
77.90	139.0
78.90	990.0
80.00	330.0
80.90	1167.0
81.80	370.0
86.00	113.0
86.90	1474.0
87.90	1717.0
91.00	166.0
92.00	1173.0
93.00	1629.0
94.00	4254.0
95.00	35512.0
96.00	2231.0
103.80	195.0
115.90	145.0
116.90	316.0
118.90	219.0
127.80	126.0
141.00	305.0
142.80	545.0
144.70	191.0
148.00	113.0
171.80	453.0
173.90	33176.0
174.90	2511.0
176.00	32584.0
177.00	2024.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

Scan 2886 (10.619 min): VU035688.D
BFB53

m/z	Abundance
40.00	157.0
44.00	1034.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53