

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111220\
 Data File : VU041216.D
 Acq On : 12 Nov 2020 14:21
 Operator : SY/MD
 Sample : L4485-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MDL-WATER-01

Quant Time: Nov 13 04:27:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM111220.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 13 04:26:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.22	114	5613	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.35	117	5681	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.74	152	2744	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.61	65	4793	0.56	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	112.00%
4) 1,2-Dichloroethane-d4	5.68	65	3961	0.46	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.00%
7) 1,2-Dichloropropane-d6	6.66	67	3340	0.48	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	96.00%
8) Toluene-d8	7.85	98	5157	0.45	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	90.00%
10) 1,1,2,2-Tetrachloroethane-	10.68	84	3231	0.47	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	94.00%

Target Compounds


					Qvalue
3) Vinyl chloride	1.61	62	252	0.031 ug/L #	18
6) Trichloroethene	6.51	95	152	0.025 ug/L	94
9) 1,2-Dibromoethane	8.87	107	108	0.024 ug/L #	86
12) 1,2,3-Trichloropropane	10.75	75	102	0.024 ug/L	94
13) 1,2-Dibromo-3-chloropropan	12.91	75	28	0.032 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111220\
Data File : VU041216.D
Acq On : 12 Nov 2020 14:21
Operator : SY/MD
Sample : L4485-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-01

Quant Time: Nov 13 04:27:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM111220.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 13 04:26:25 2020
Response via : Initial Calibration

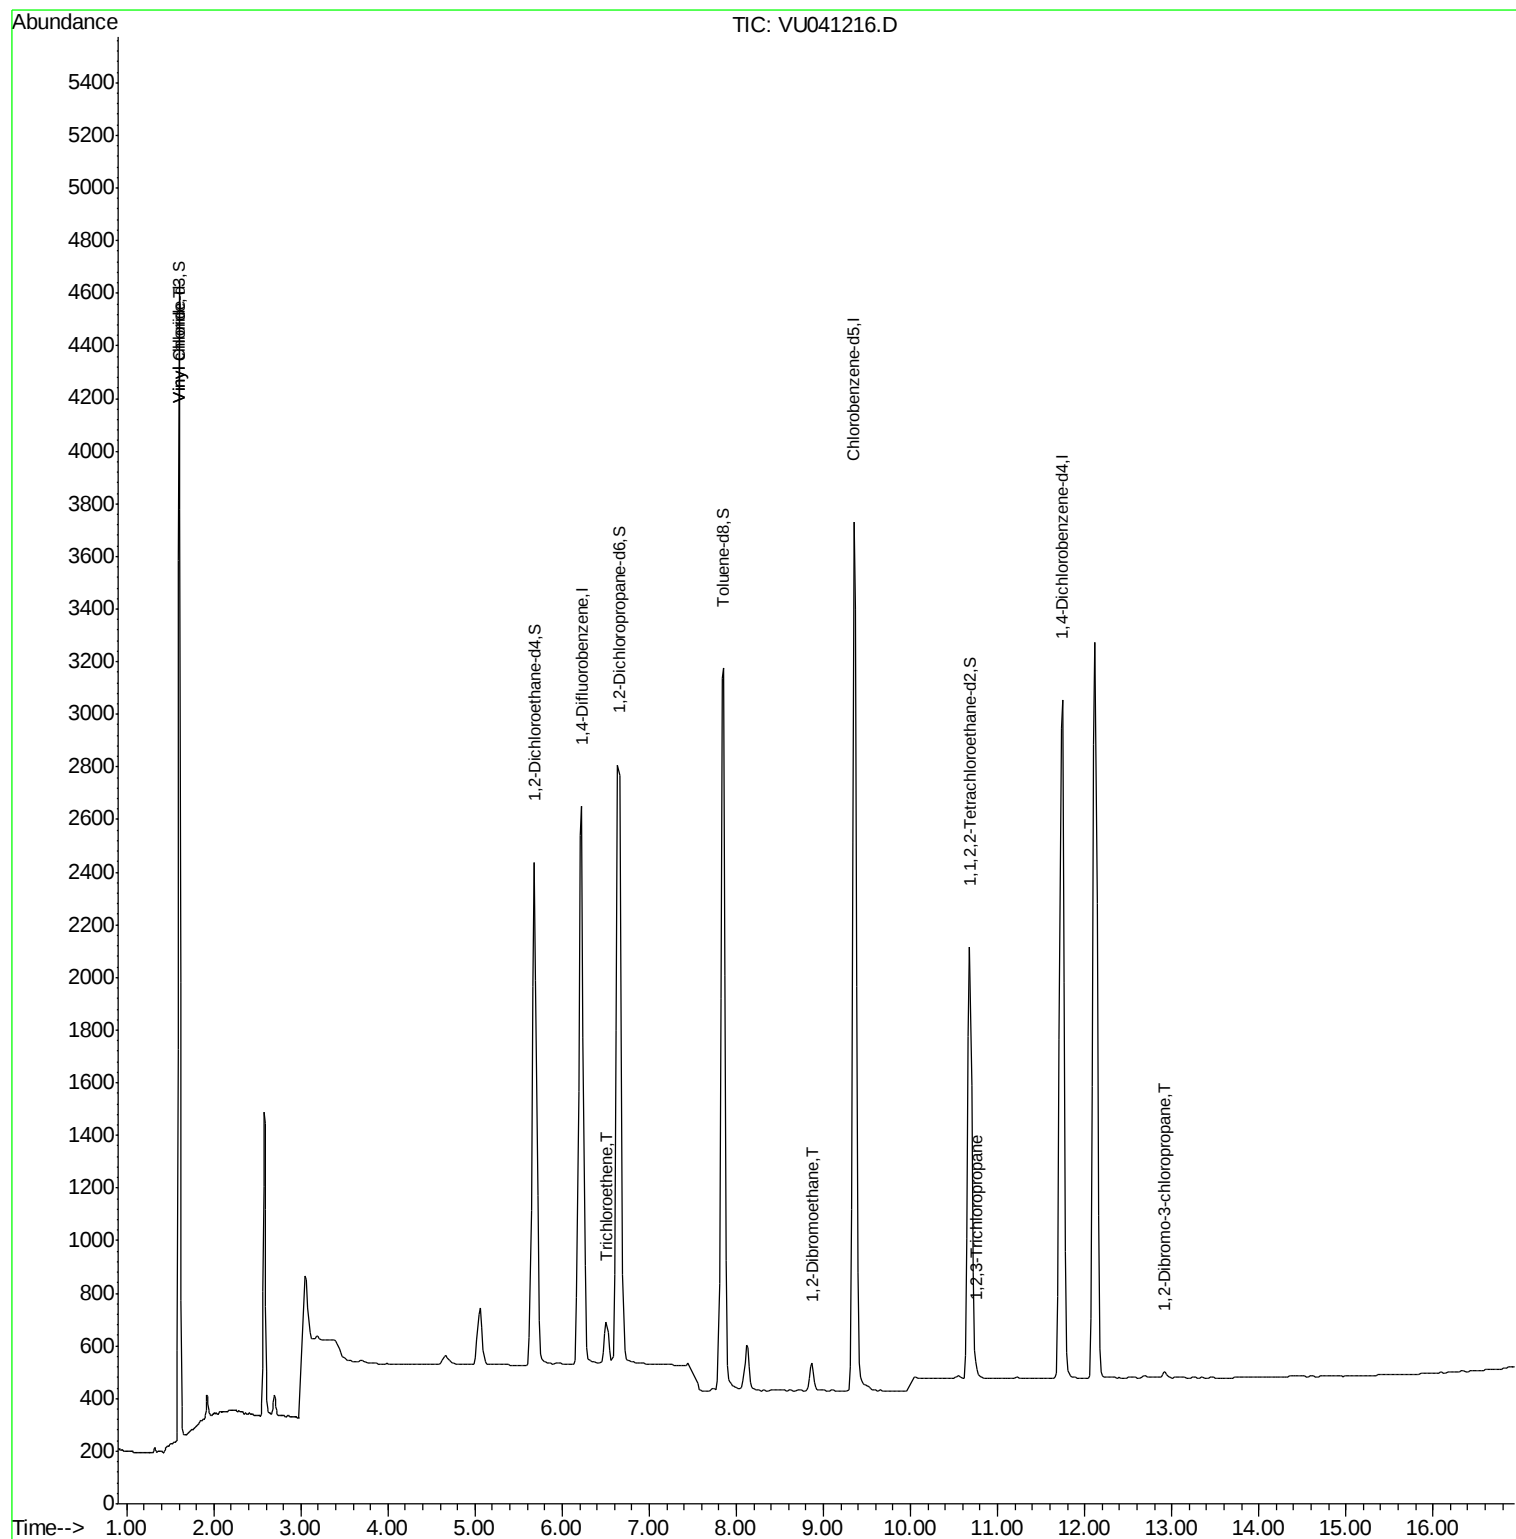

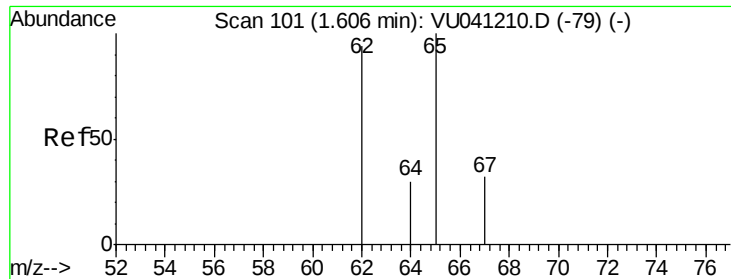

#3

Vinyl chloride

Concen: 0.031 ug/L

RT: 1.61 min Scan# 101

Delta R.T. -0.00 min

Lab File: VU041216.D

Acq: 12 Nov 2020 14:21

Instrument :

MSVOA_U

ClientSampleId :





MDL-WATER-01

Tot Ion: 62 Resp: 252

Ion Ratio Lower Upper

62 100

64 81.4 23.9 44.3#

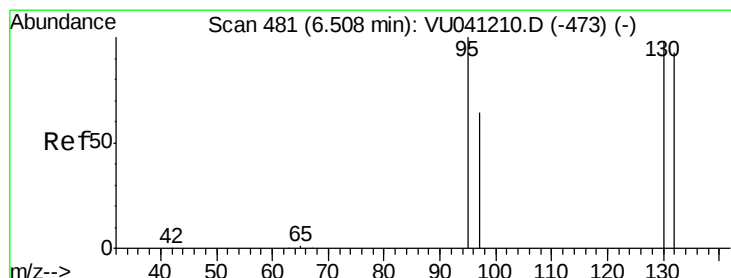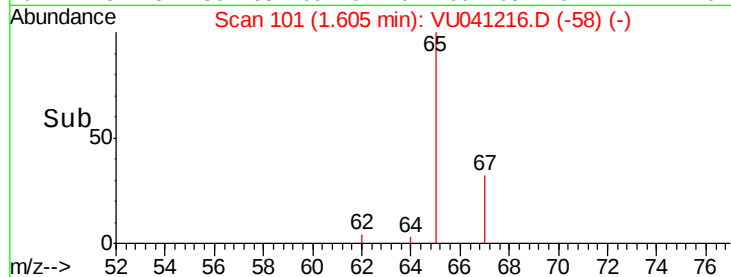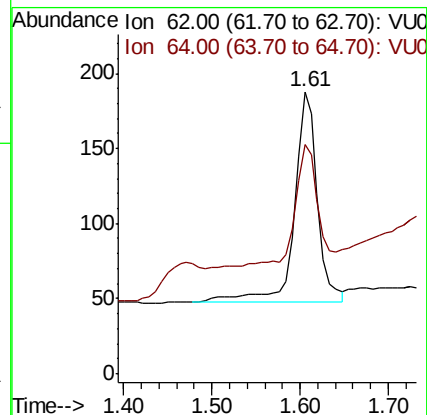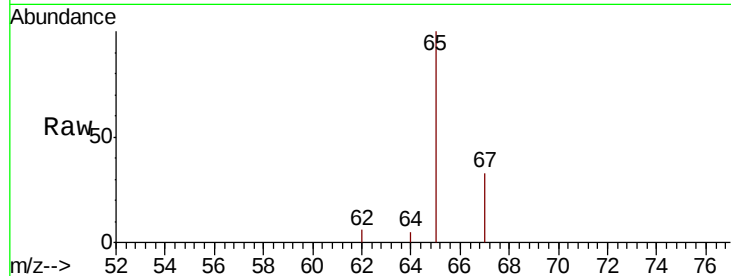

#6

Trichloroethene

Concen: 0.025 ug/L

RT: 6.51 min Scan# 481

Delta R.T. -0.00 min

Lab File: VU041216.D

Acq: 12 Nov 2020 14:21

Tgt Ion: 95 Resp: 152




Ion Ratio Lower Upper


95 100

97 82.2 46.0 85.4

132 94.4 65.3 121.3

130 97.8 68.7 127.7

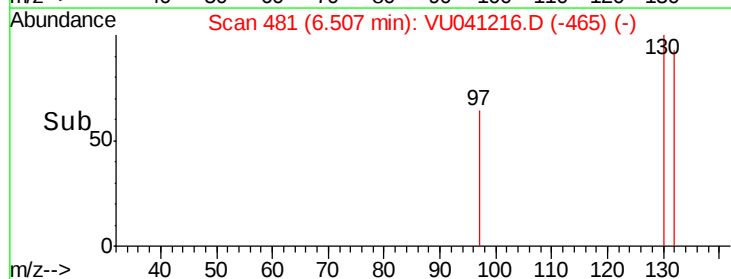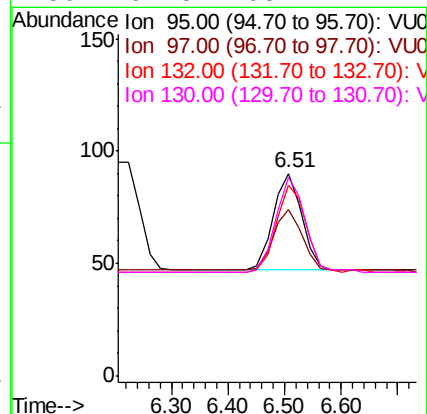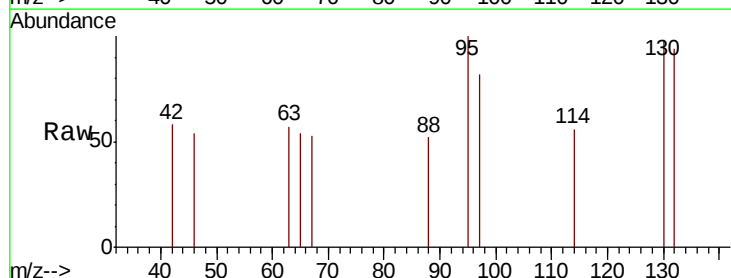

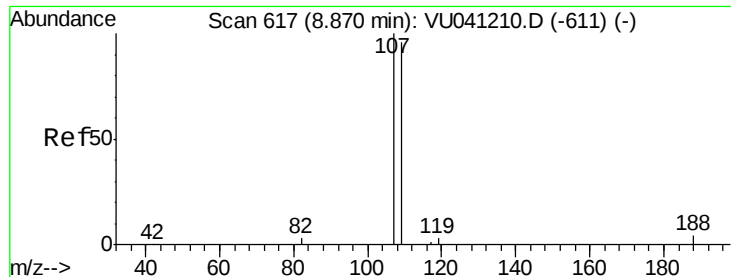

#9

1,2-Dibromoethane

Concen: 0.024 ug/L

RT: 8.87 min Scan# 617

Delta R.T. -0.00 min

Lab File: VU041216.D

Acq: 12 Nov 2020 14:21

Instrument :

MSVOA_U

ClientSampleId :

MDL-WATER-01


Tot Ion:107 Resp: 108

Ion Ratio Lower Upper

107 100

109 94.9 67.7 125.7




188 60.3 7.0 10.6#

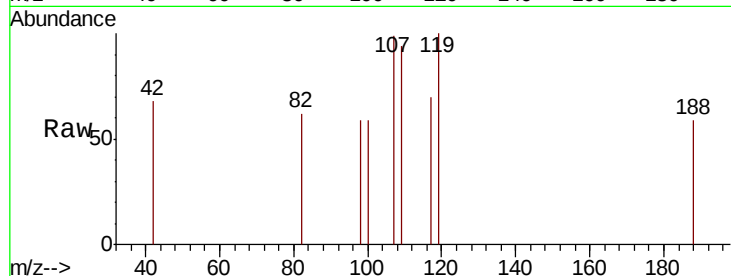

Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

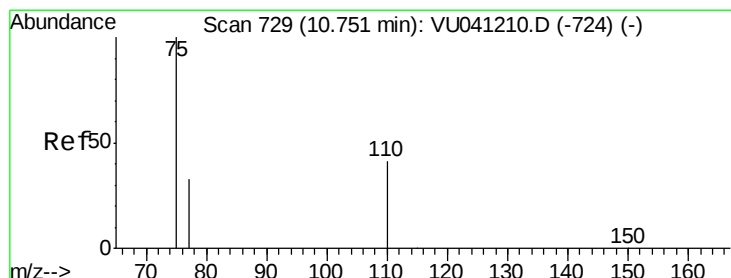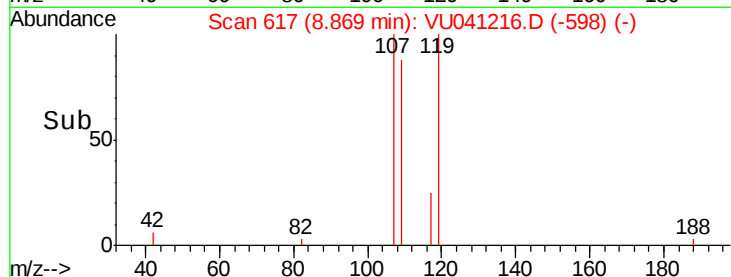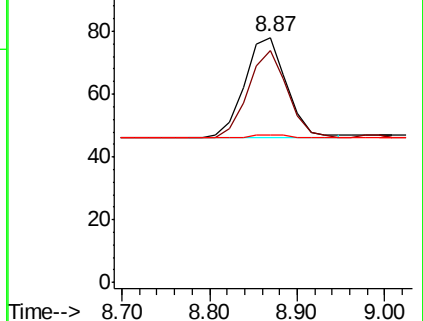

#12

1,2,3-Trichloropropane

Concen: 0.024 ug/L

RT: 10.75 min Scan# 729

Delta R.T. -0.00 min

Lab File: VU041216.D

Acq: 12 Nov 2020 14:21


Tgt Ion: 75 Resp: 102

Ion Ratio Lower Upper

75 100

110 36.3 31.0 46.4



77 28.4 26.7 40.1

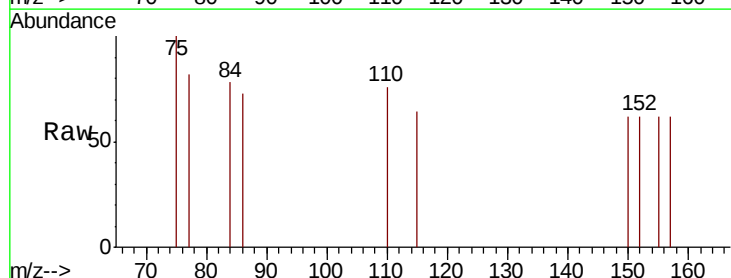


Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VU0

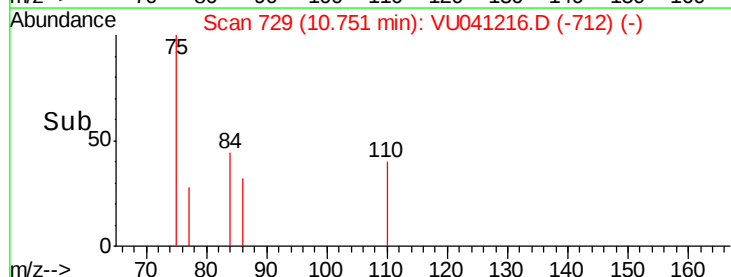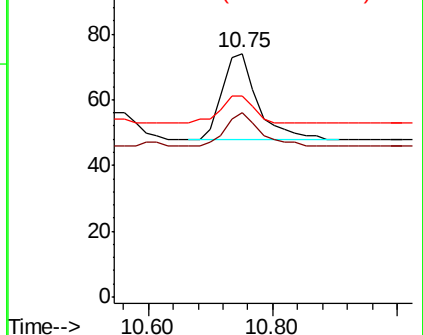

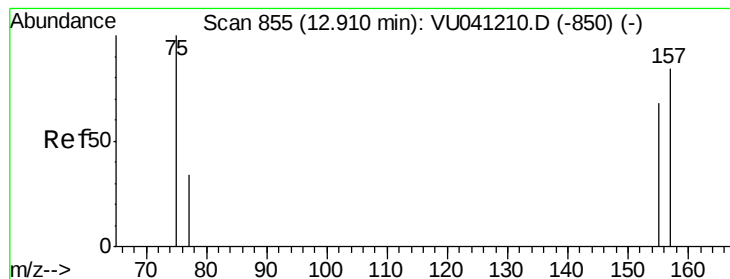

#13

1,2-Dibromo-3-chloropropane

Concen: 0.032 ug/L

RT: 12.91 min Scan# 855

Delta R.T. -0.00 min

Lab File: VU041216.D


Acq: 12 Nov 2020 14:21

Instrument :

MSVOA_U

ClientSampleId :

MDL-WATER-01

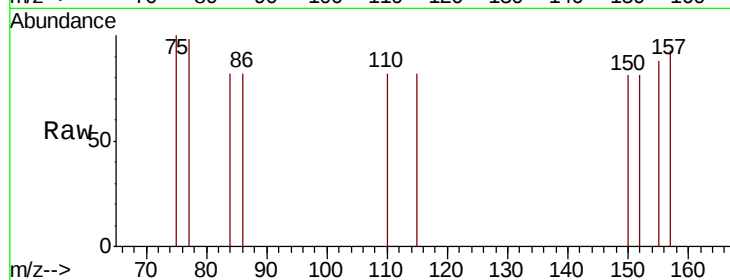


Tot Ion: 75 Resp: 28

Ion Ratio Lower Upper

75 100

157 93.0 68.7 103.1

155 87.7 58.9 88.3

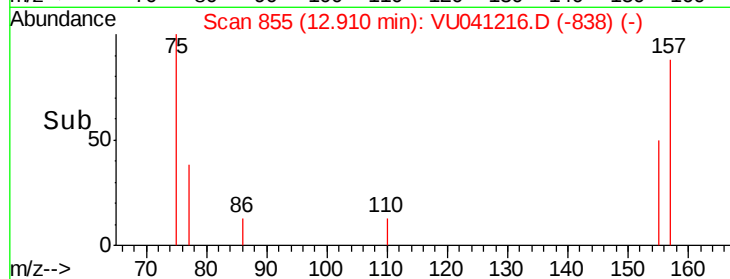

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 157.00 (156.70 to 157.70): V

Ion 155.00 (154.70 to 155.70): V

