

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111221\
 Data File : VU045758.D
 Acq On : 12 Nov 2021 10:45
 Operator : SY/MD
 Sample : VU1112WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1112WBL01

Quant Time: Nov 15 05:17:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.378	168	117203	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	219124	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	225528	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.815	152	105626	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	96650	55.063	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	110.120%
35) Dibromofluoromethane	5.292	113	76920	52.578	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.160%
50) Toluene-d8	7.899	98	287683	52.882	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	105.760%
62) 4-Bromofluorobenzene	10.635	95	106265	48.713	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.420%
Target Compounds						
						Qvalue
16) Acetone	2.629	43	514	0.575	ug/l	93
31) Cyclohexane	5.375	56	2623	1.024	ug/l #	1
36) 1,1-Dichloropropene	5.375	75	10807	5.058	ug/l #	48
38) Carbon Tetrachloride	5.375	117	12448	5.779	ug/l #	16
59) 2-Hexanone	8.687	43	176	7.614	ug/l #	21
76) 1,2,3-Trichloropropane	10.635	75	55398	17.295	ug/l #	42
81) trans-1,4-Dichloro-2-b...	10.635	75	55398	56.258	ug/l #	12
95) Naphthalene	14.095	128	737	1.113	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111221\
Data File : VU045758.D
Acq On : 12 Nov 2021 10:45
Operator : SY/MD
Sample : VU1112WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Quant Time: Nov 15 05:17:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 05 13:35:16 2021
Response via : Initial Calibration




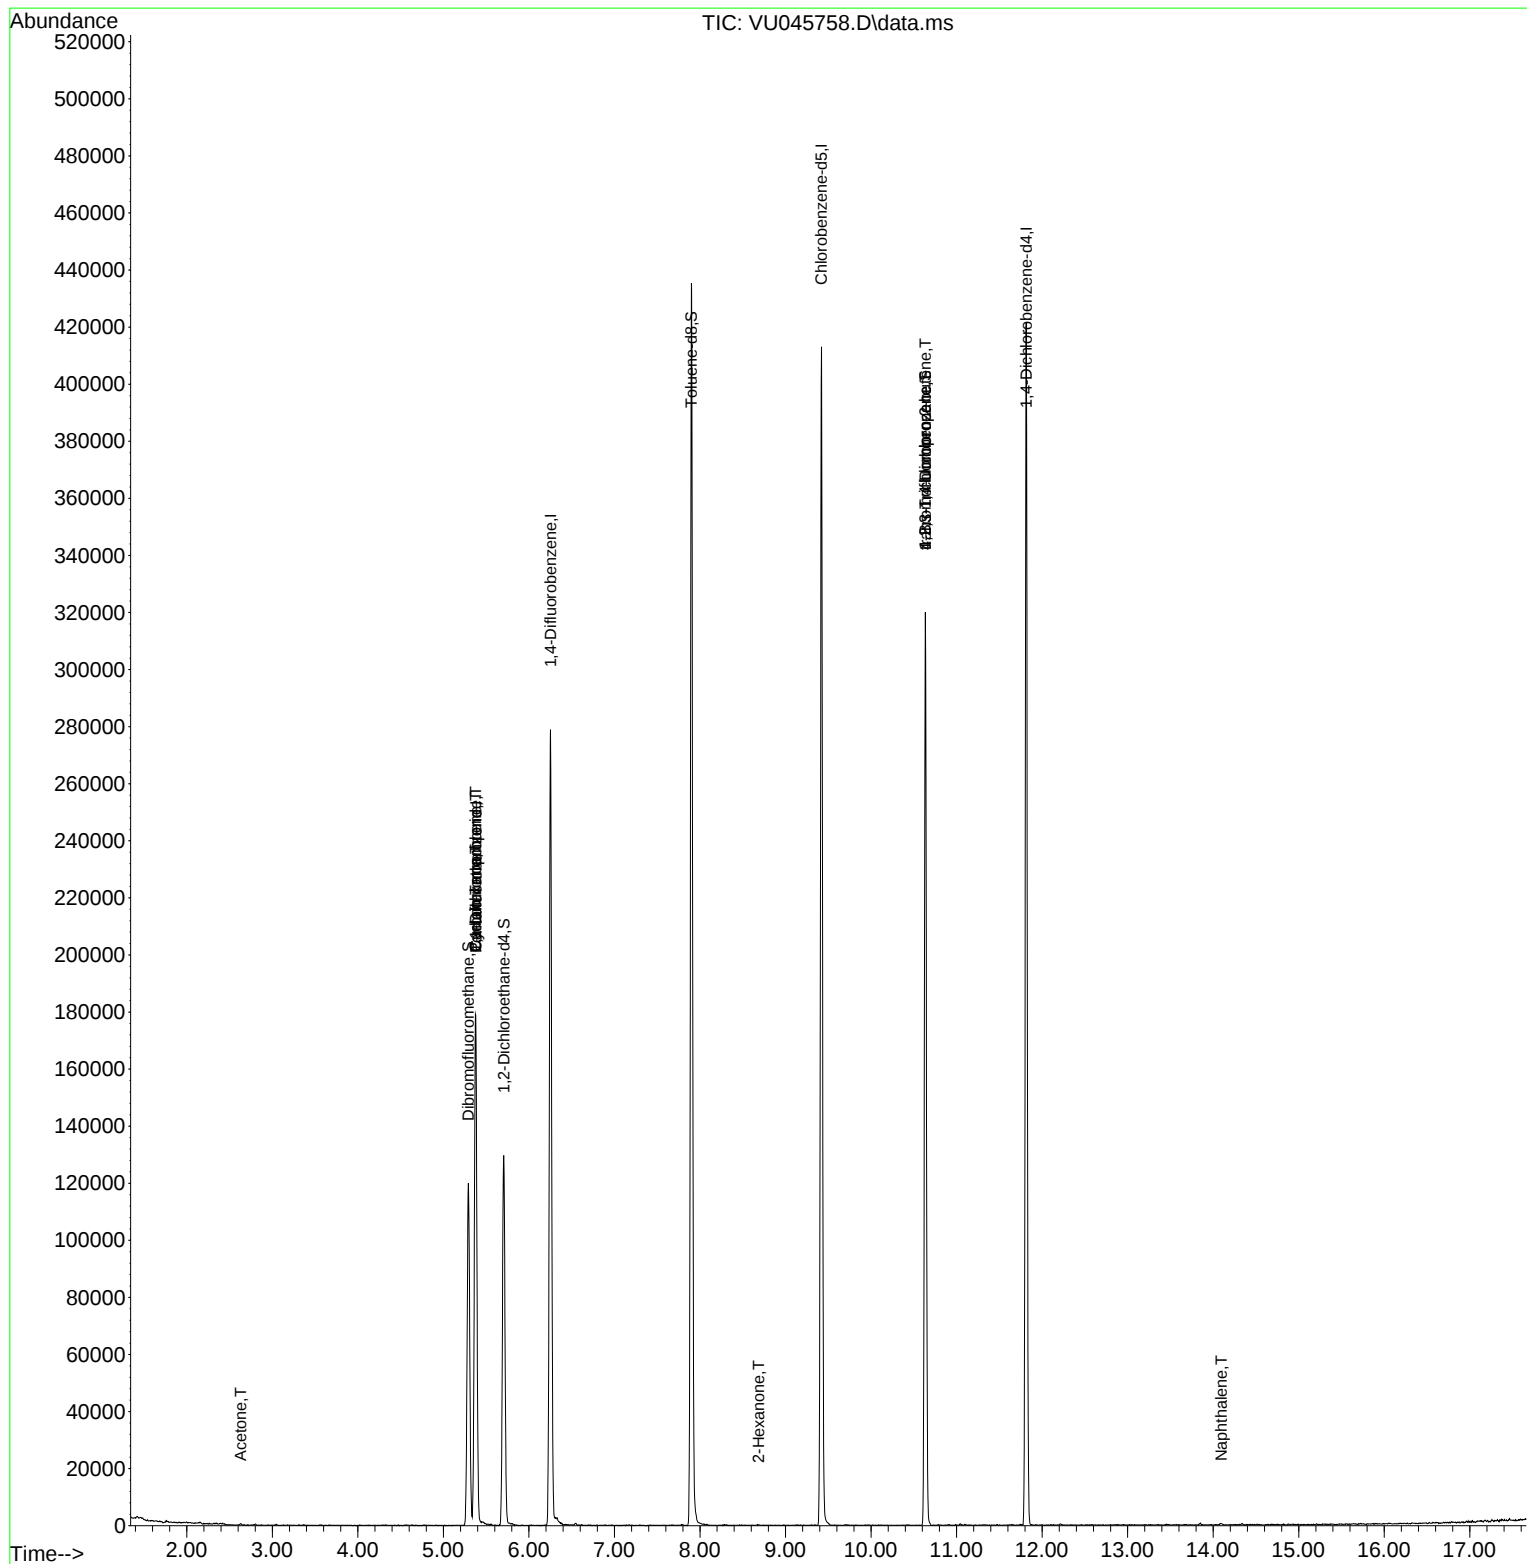




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.378 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45




Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01


Tgt Ion:168 Resp: 117203
Ion Ratio Lower Upper
168 100
99 65.5 51.0 76.6

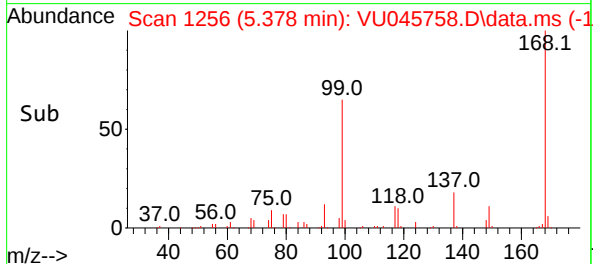

#16
Acetone
Concen: 0.575 ug/l
RT: 2.629 min Scan# 401
Delta R.T. 0.006 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Tgt Ion: 43 Resp: 514
Ion Ratio Lower Upper
43 100
58 28.7 26.2 39.2


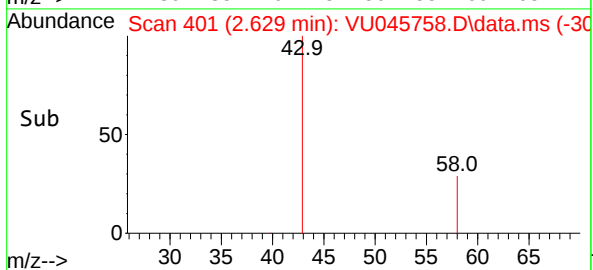

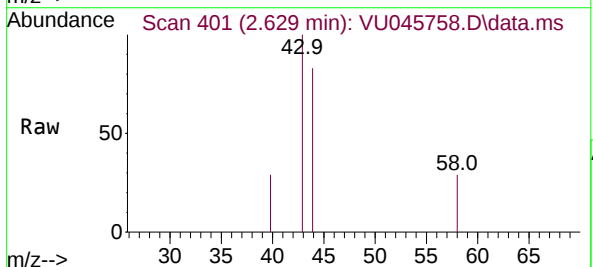


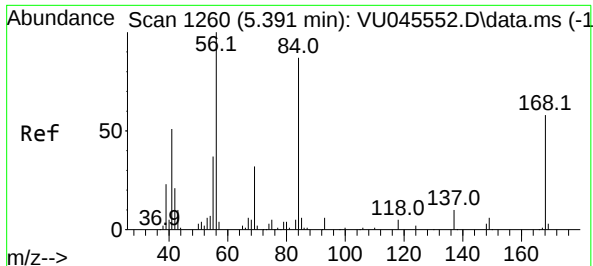

#31
Cyclohexane
Concen: 1.024 ug/l
RT: 5.375 min Scan# 11
Delta R.T. -0.016 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45




Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01


Tgt Ion: 56 Resp: 2623
Ion Ratio Lower Upper
56 100
69 171.0 26.4 39.6#
84 136.0 68.4 102.6#

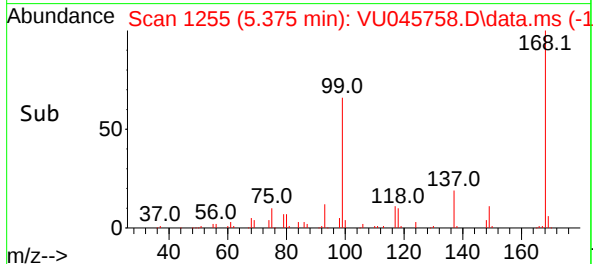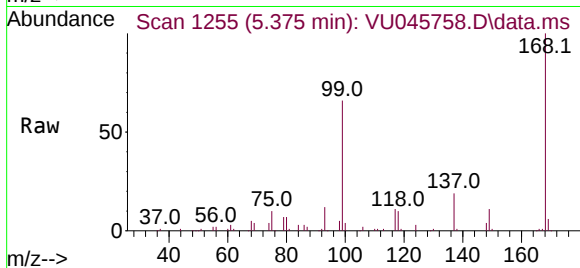

#33
1,2-Dichloroethane-d4
Concen: 55.063 ug/l
RT: 5.706 min Scan# 1358
Delta R.T. 0.003 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Tgt Ion: 65 Resp: 96650
Ion Ratio Lower Upper
65 100
67 53.5 0.0 105.8

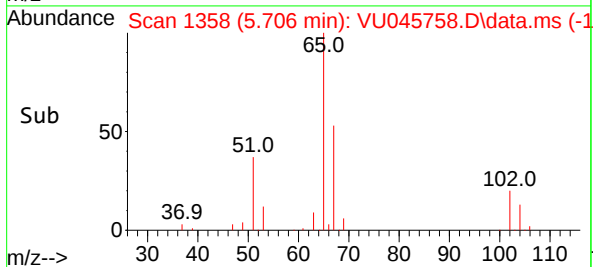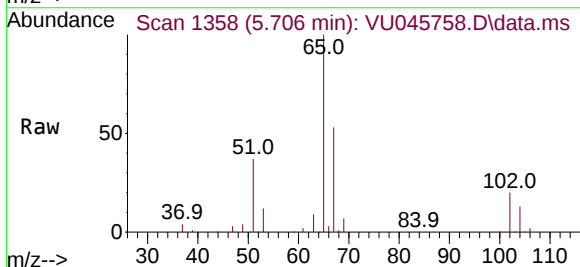

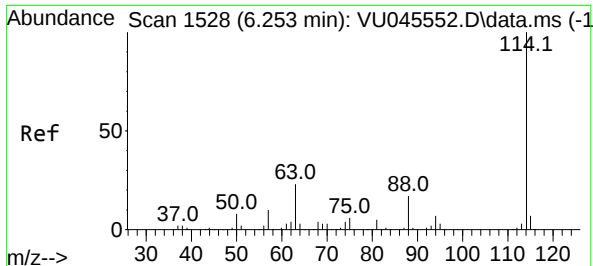

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 11

Delta R.T. -0.000 min

Lab File: VU045758.D

Acq: 12 Nov 2021 10:45

Instrument :

MSVOA_U

ClientSampleId :

VU1112WBL01





Tgt Ion:114 Resp: 219124

Ion Ratio Lower Upper

114 100

63 22.6 0.0 45.6

88 17.0 0.0 33.8

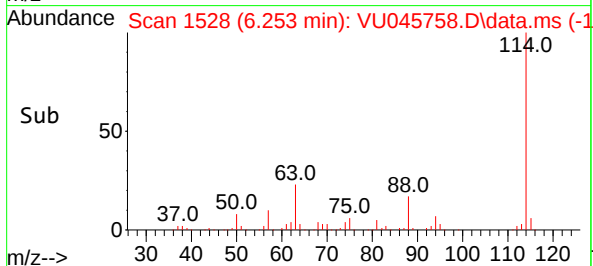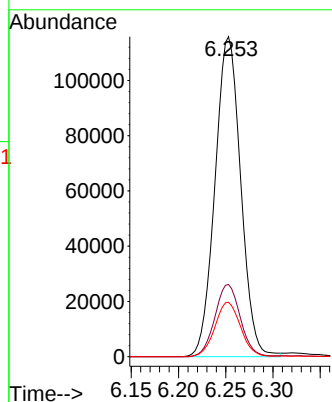

#35

Dibromofluoromethane

Concen: 52.578 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. -0.000 min

Lab File: VU045758.D

Acq: 12 Nov 2021 10:45




Tgt Ion:113 Resp: 76920


Ion Ratio Lower Upper

113 100

111 102.8 82.8 124.2

192 17.9 14.8 22.2

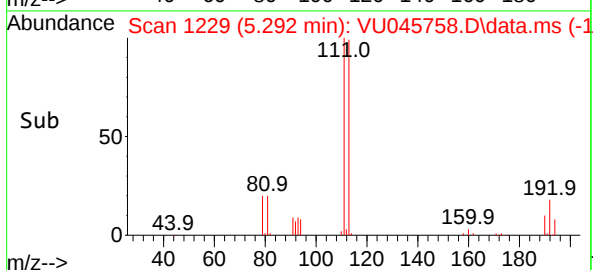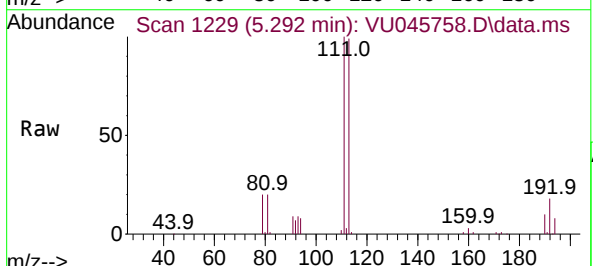

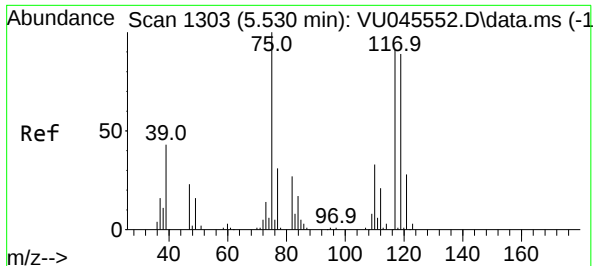

#36

1,1-Dichloropropene

Concen: 5.058 ug/l

RT: 5.375 min Scan# 1255

Delta R.T. -0.154 min

Lab File: VU045758.D

Acq: 12 Nov 2021 10:45

Instrument :

MSVOA_U

ClientSampleId :

VU1112WBL01





Tgt Ion: 75 Resp: 10807

Ion Ratio Lower Upper

75 100

110 6.7 16.7 50.0#

77 0.0 25.0 37.4#

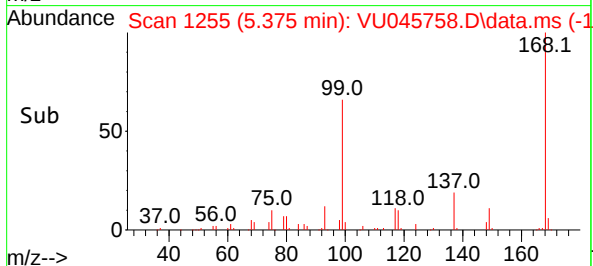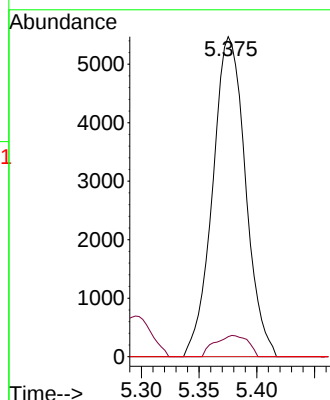

#38

Carbon Tetrachloride

Concen: 5.779 ug/l

RT: 5.375 min Scan# 1255

Delta R.T. -0.154 min

Lab File: VU045758.D

Acq: 12 Nov 2021 10:45




Tgt Ion: 117 Resp: 12448


Ion Ratio Lower Upper

117 100

119 5.8 77.4 116.0#

121 0.0 24.8 37.2#


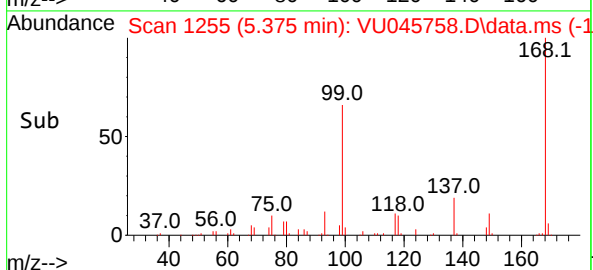
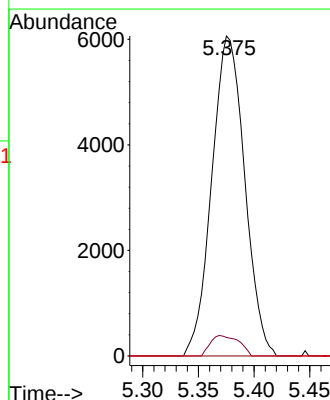
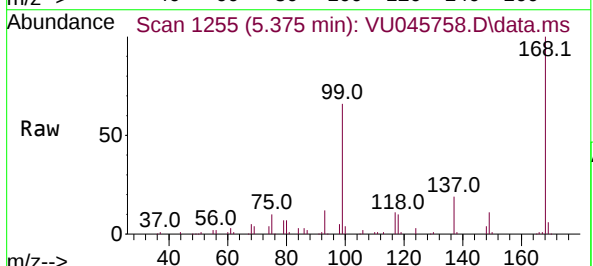


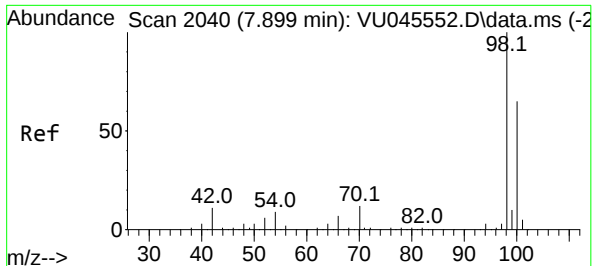

#50
Toluene-d8
Concen: 52.882 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. -0.000 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45




Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01


Tgt Ion: 98 Resp: 287683
Ion Ratio Lower Upper
98 100
100 65.7 52.5 78.7

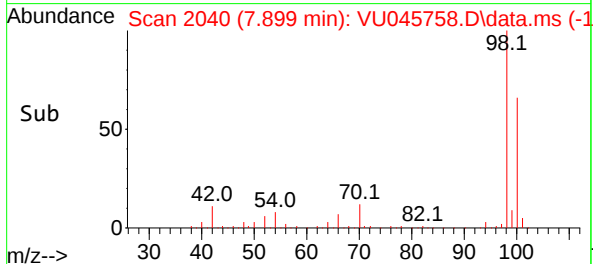

#59
2-Hexanone
Concen: 7.614 ug/l
RT: 8.687 min Scan# 2285
Delta R.T. 0.003 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Tgt Ion: 43 Resp: 176
Ion Ratio Lower Upper
43 100
58 0.0 29.5 88.6#


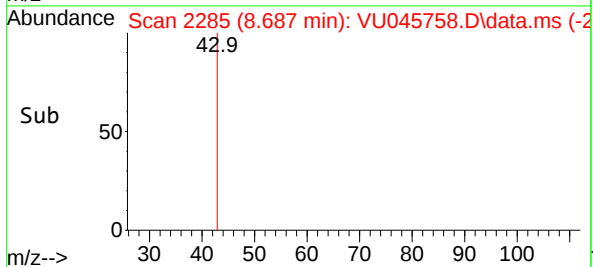

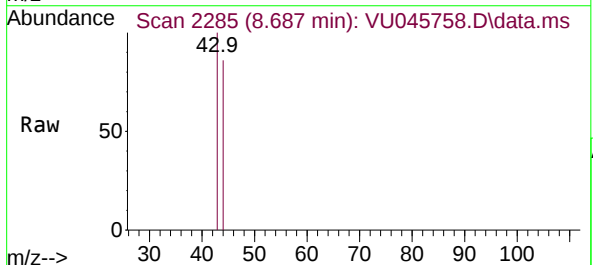


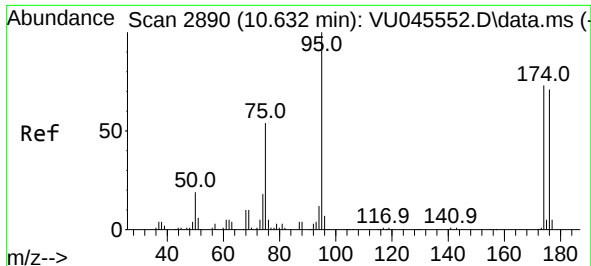

#62
4-Bromofluorobenzene
Concen: 48.713 ug/l
RT: 10.635 min Scan# 2890
Delta R.T. 0.003 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45




Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01


Tgt Ion: 95 Resp: 106265
Ion Ratio Lower Upper
95 100
174 75.6 0.0 141.8
176 71.6 0.0 138.2

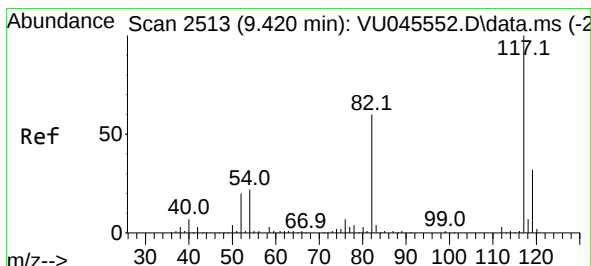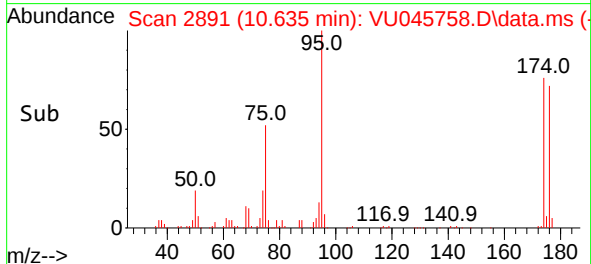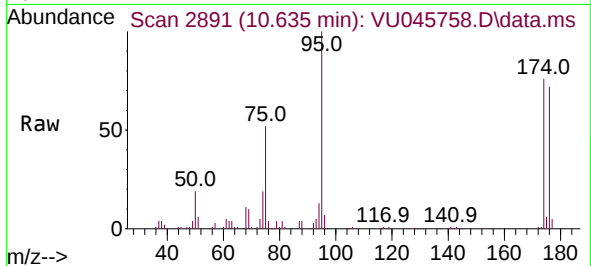

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Tgt Ion: 117 Resp: 225528
Ion Ratio Lower Upper
117 100
82 57.4 47.8 71.8
119 32.0 25.8 38.8

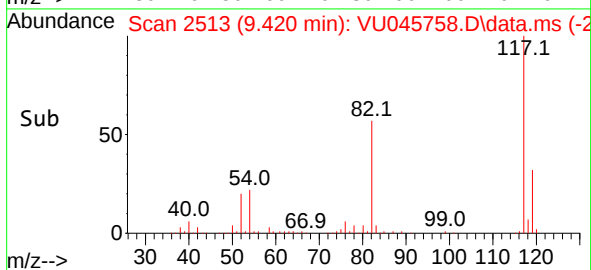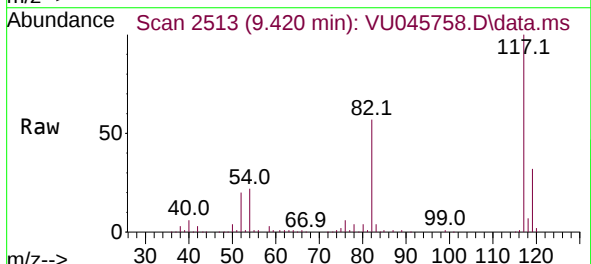

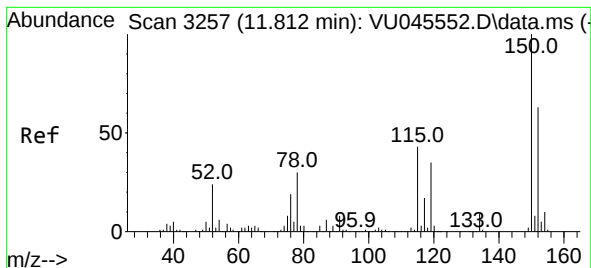

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.815 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU045758.D

Acq: 12 Nov 2021 10:45

Instrument :

MSVOA_U

ClientSampleId :

VU1112WBL01





Tgt Ion:152 Resp: 105626

Ion Ratio Lower Upper

152 100

115 62.7 42.7 128.1

150 159.2 0.0 346.8

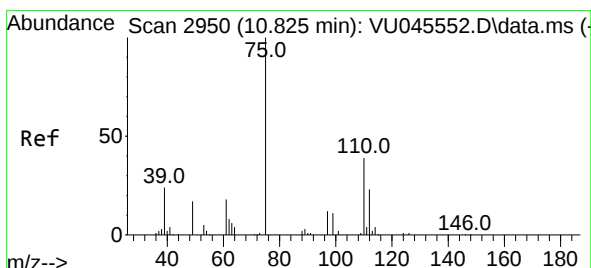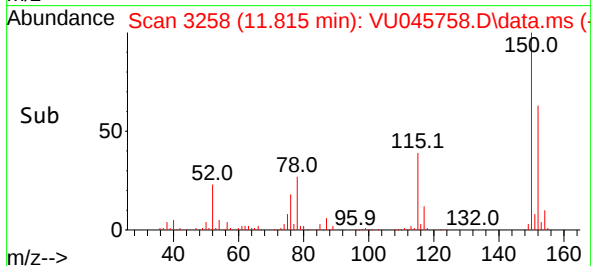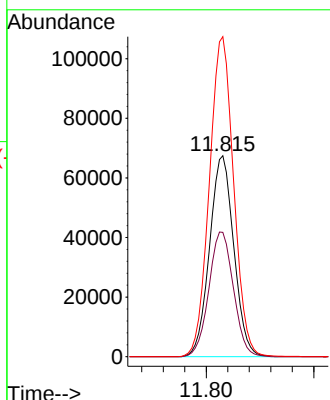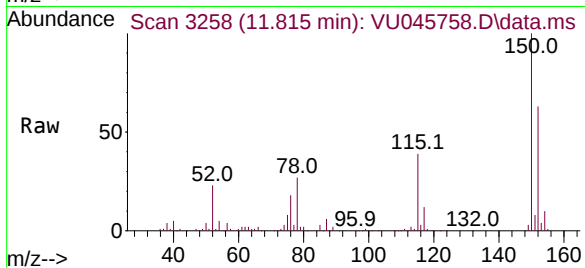

#76

1,2,3-Trichloropropane

Concen: 17.295 ug/l

RT: 10.635 min Scan# 2891

Delta R.T. -0.190 min

Lab File: VU045758.D




Acq: 12 Nov 2021 10:45


Tgt Ion: 75 Resp: 55398

Ion Ratio Lower Upper

75 100

77 1.1 17.1 51.3#


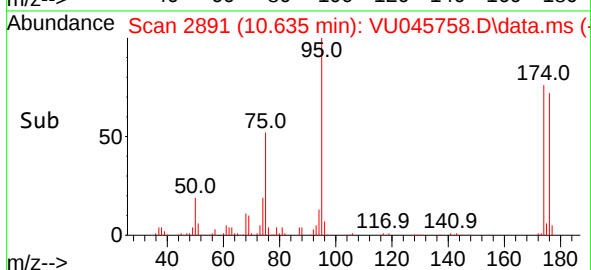
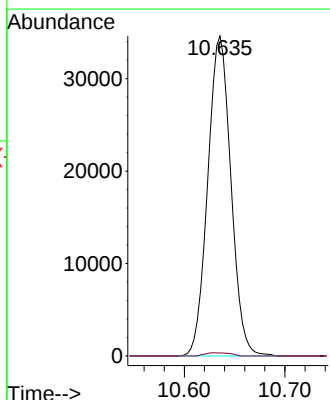
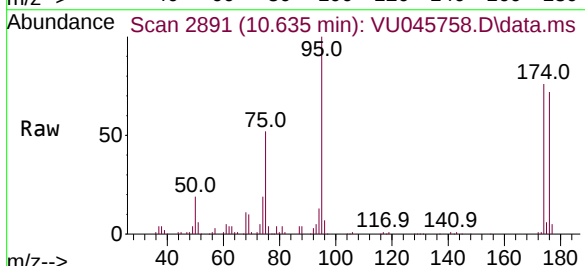


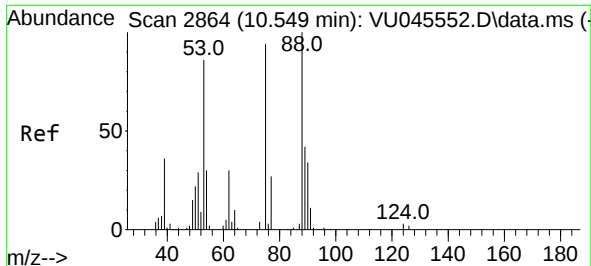

#81
trans-1,4-Dichloro-2-butene
Concen: 56.258 ug/l
RT: 10.635 min Scan# 21
Delta R.T. 0.086 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Instrument :
MSVOA_U
ClientSampleId :
VU1112WBL01

Tgt Ion: 75 Resp: 55398
Ion Ratio Lower Upper
75 100
53 0.0 76.2 114.4#
89 0.0 34.0 51.0#

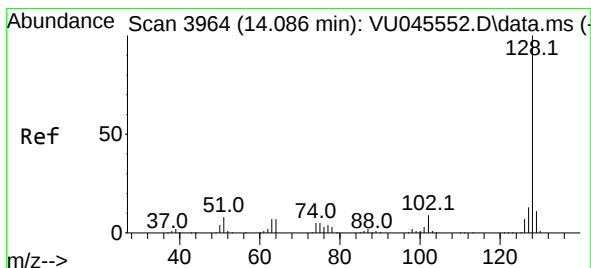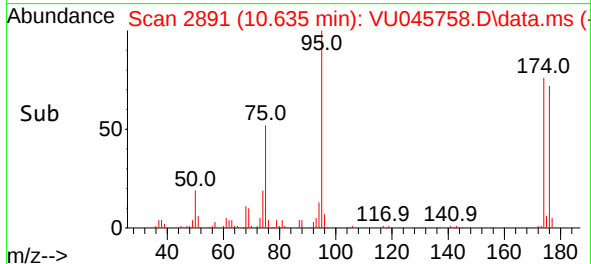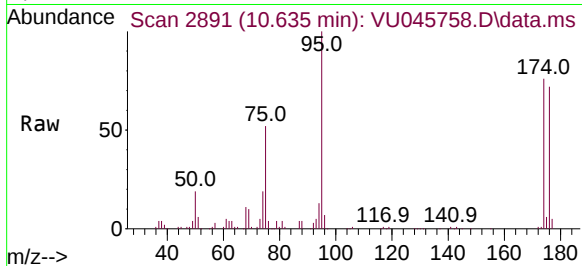

#95
Naphthalene
Concen: 1.113 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.009 min
Lab File: VU045758.D
Acq: 12 Nov 2021 10:45

Tgt Ion: 128 Resp: 737
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 13.0#

