

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111221\  
Data File : VU045762.D  
Acq On : 12 Nov 2021 12:29  
Operator : SY/MD  
Sample : M4606-20 40X  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
DUP-02-20211109

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M

Title : SW846 8260

Signal : TIC: VU045762.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.292       | 1214          | 1229        | 1243         | rBV2     | 115538         | 245404        | 32.79%          | 6.113%        |
| 2         | 5.375       | 1243          | 1255        | 1273         | rVB      | 176584         | 362298        | 48.40%          | 9.025%        |
| 3         | 5.707       | 1342          | 1358        | 1377         | rBV      | 129275         | 260154        | 34.76%          | 6.481%        |
| 4         | 6.253       | 1511          | 1528        | 1545         | rBV      | 276021         | 516946        | 69.07%          | 12.878%       |
| 5         | 7.903       | 2026          | 2041        | 2072         | rBV      | 426895         | 748488        | 100.00%         | 18.646%       |
| 6         | 9.420       | 2498          | 2513        | 2532         | rBV      | 409788         | 679103        | 90.73%          | 16.917%       |
| 7         | 10.636      | 2878          | 2891        | 2912         | rBV      | 323638         | 511427        | 68.33%          | 12.740%       |
| 8         | 11.816      | 3245          | 3258        | 3279         | rVB      | 431544         | 690471        | 92.25%          | 17.200%       |




Sum of corrected areas: 4014291

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111221\  
Data File : VU045762.D  
Acq On : 12 Nov 2021 12:29  
Operator : SY/MD  
Sample : M4606-20 40X  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
DUP-02-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

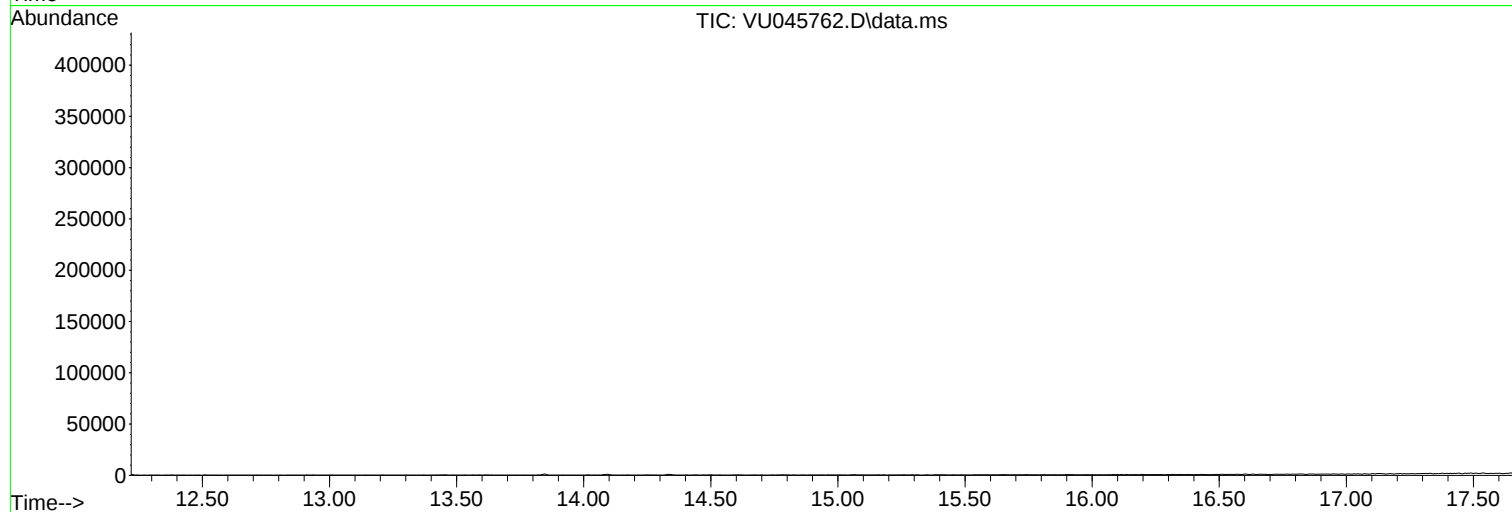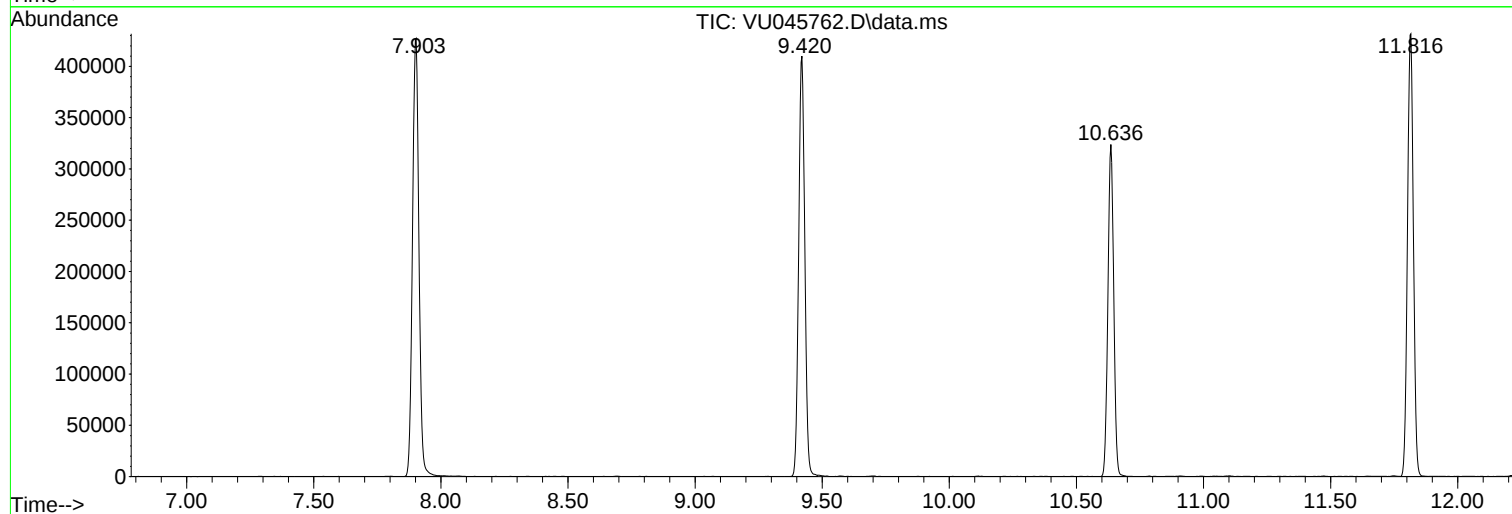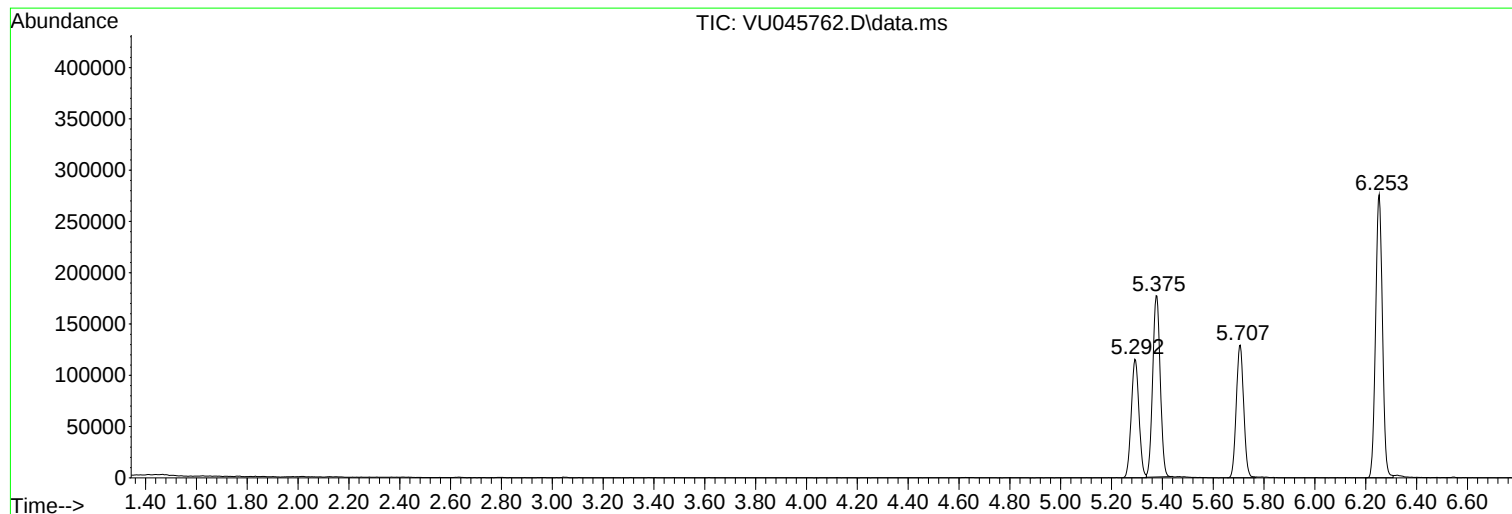

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111221\  
Data File : VU045762.D  
Acq On : 12 Nov 2021 12:29  
Operator : SY/MD  
Sample : M4606-20 40X  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
DUP-02-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU111221\  
Data File : VU045762.D  
Acq On : 12 Nov 2021 12:29  
Operator : SY/MD  
Sample : M4606-20 40X  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
DUP-02-20211109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|