
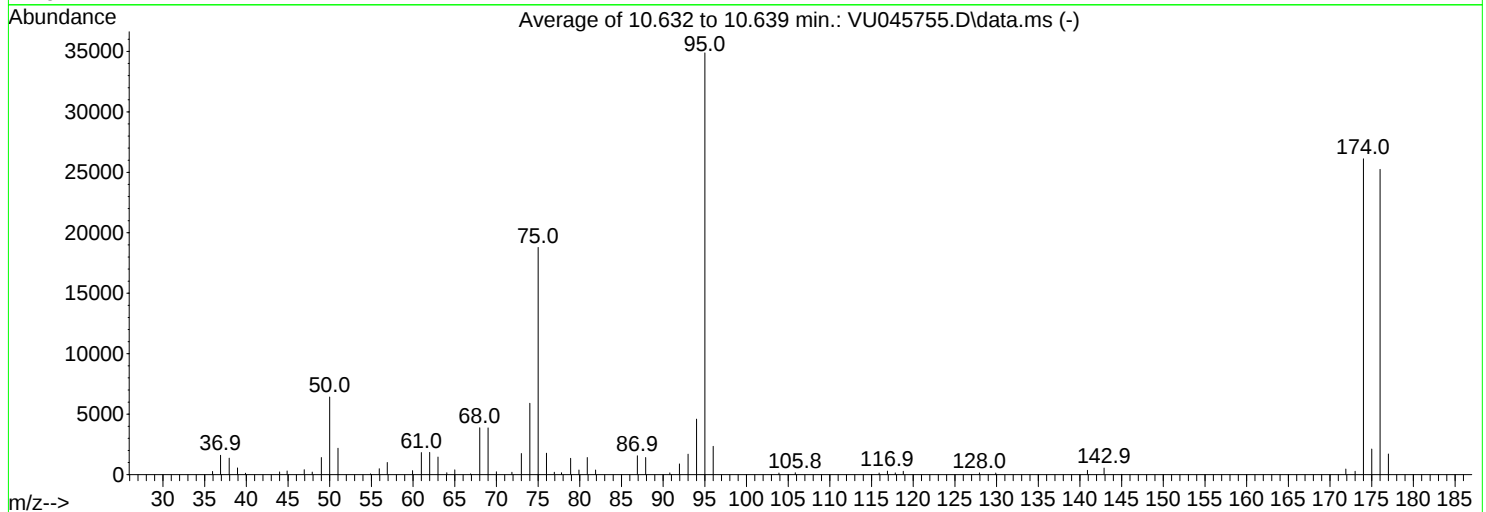


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111221\
Data File : VU045755.D
Acq On : 12 Nov 2021 09:02
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Title : SW846 8260
Last Update : Fri Nov 05 13:35:16 2021

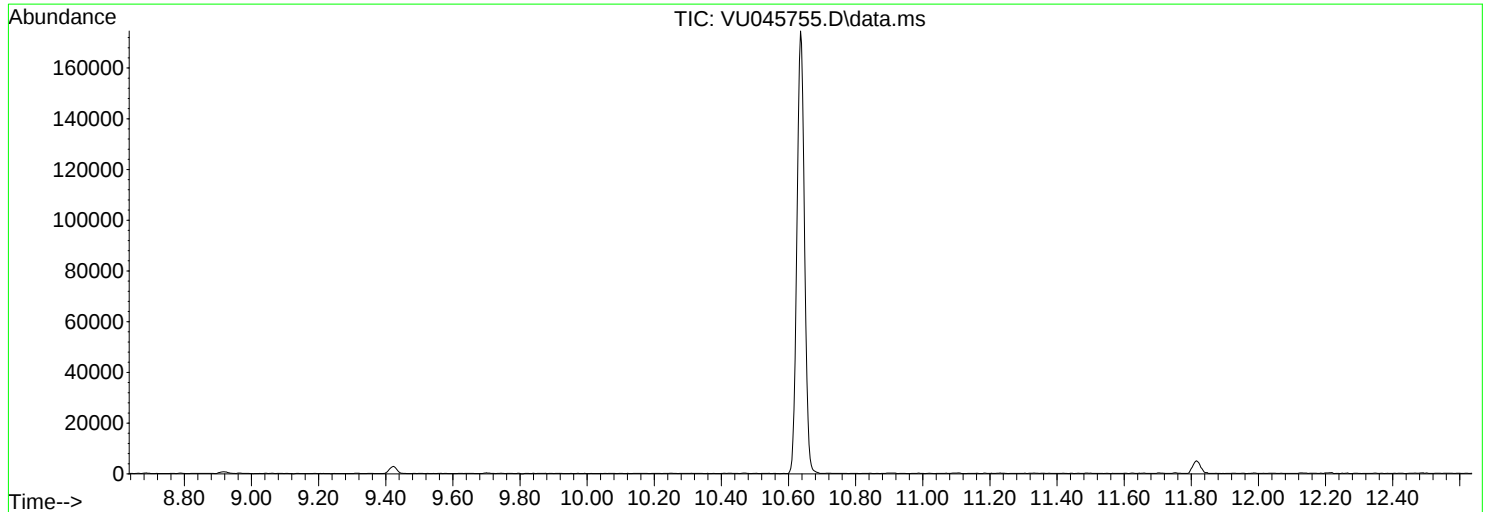

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	6423	PASS
75	95	30	60	53.9	18787	PASS
95	95	100	100	100.0	34880	PASS
96	95	5	9	6.7	2347	PASS
173	174	0.00	2	1.1	285	PASS
174	95	50	100	74.9	26123	PASS
175	174	5	9	8.1	2124	PASS
176	174	95	101	96.6	25245	PASS
177	176	5	9	6.8	1705	PASS