


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111318\  
Data File : VU028080.D  
Acq On : 13 Nov 2018 10:02  
Operator : MD/SY  
Sample : BFB  
Misc : 5.0mL/MSVOA U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U110218W.M  
Title : SW846 8260  
Last Update : Fri Nov 02 02:28:20 2018

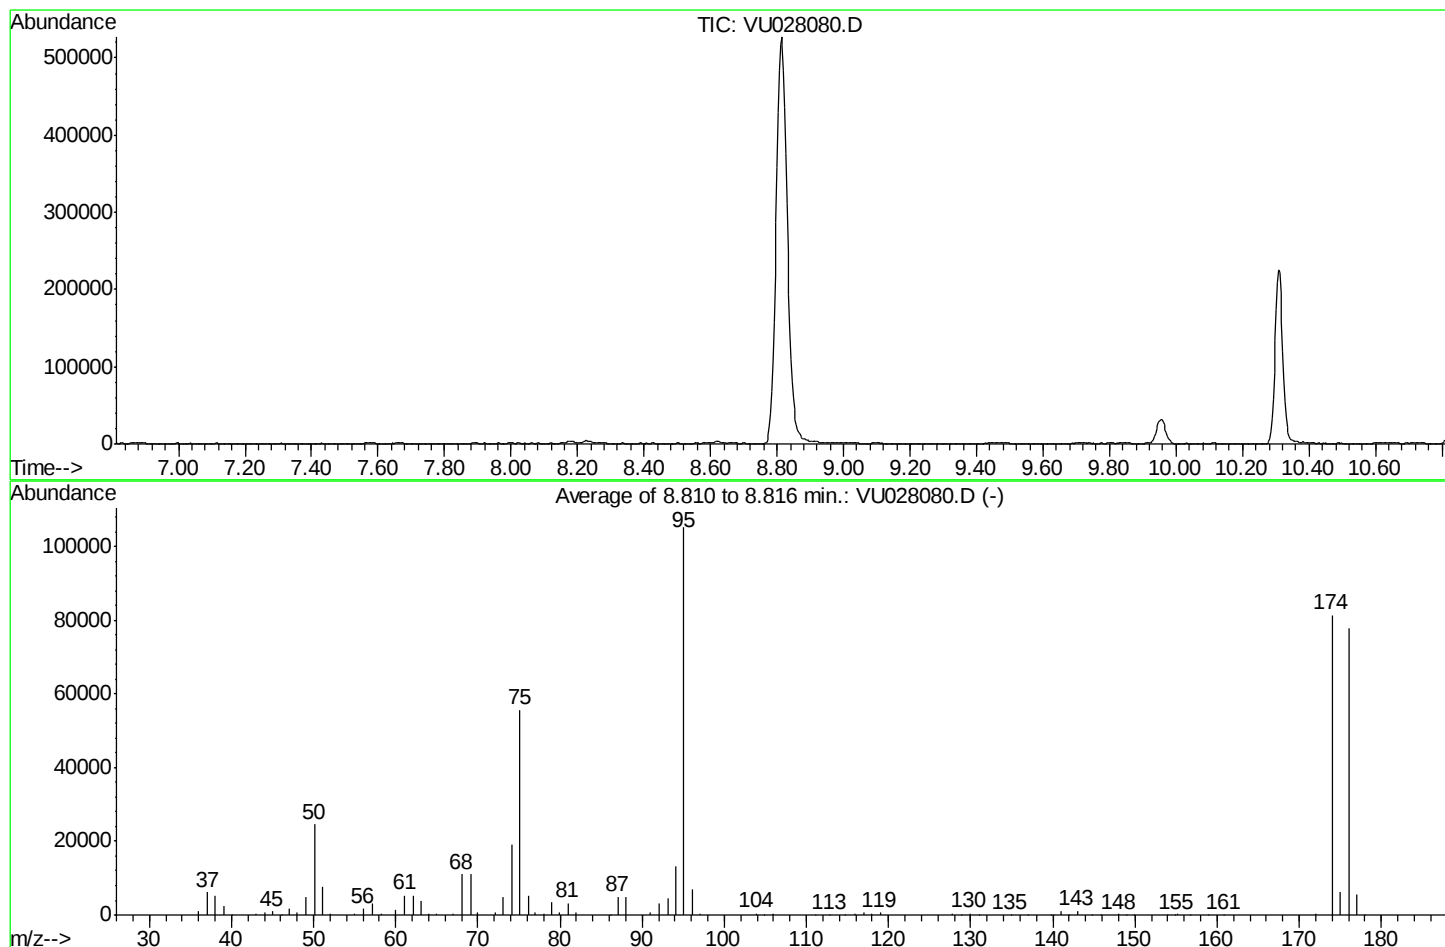

AutoFind: Scans 2375, 2376, 2377; Background Corrected with Scan 2358

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 23.3      | 24554   | PASS             |
| 75          | 95           | 30           | 60           | 52.9      | 55704   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 105216  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 6896    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 77.4      | 81429   | PASS             |
| 175         | 174          | 5            | 9            | 7.8       | 6367    | PASS             |
| 176         | 174          | 95           | 101          | 95.6      | 77834   | PASS             |
| 177         | 176          | 5            | 9            | 7.3       | 5702    | PASS             |