


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111319\
 Data File : VU035700.D
 Acq On : 13 Nov 2019 08:13
 Operator : JC/SP
 Sample : BFB26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 14 07:39:31 2019

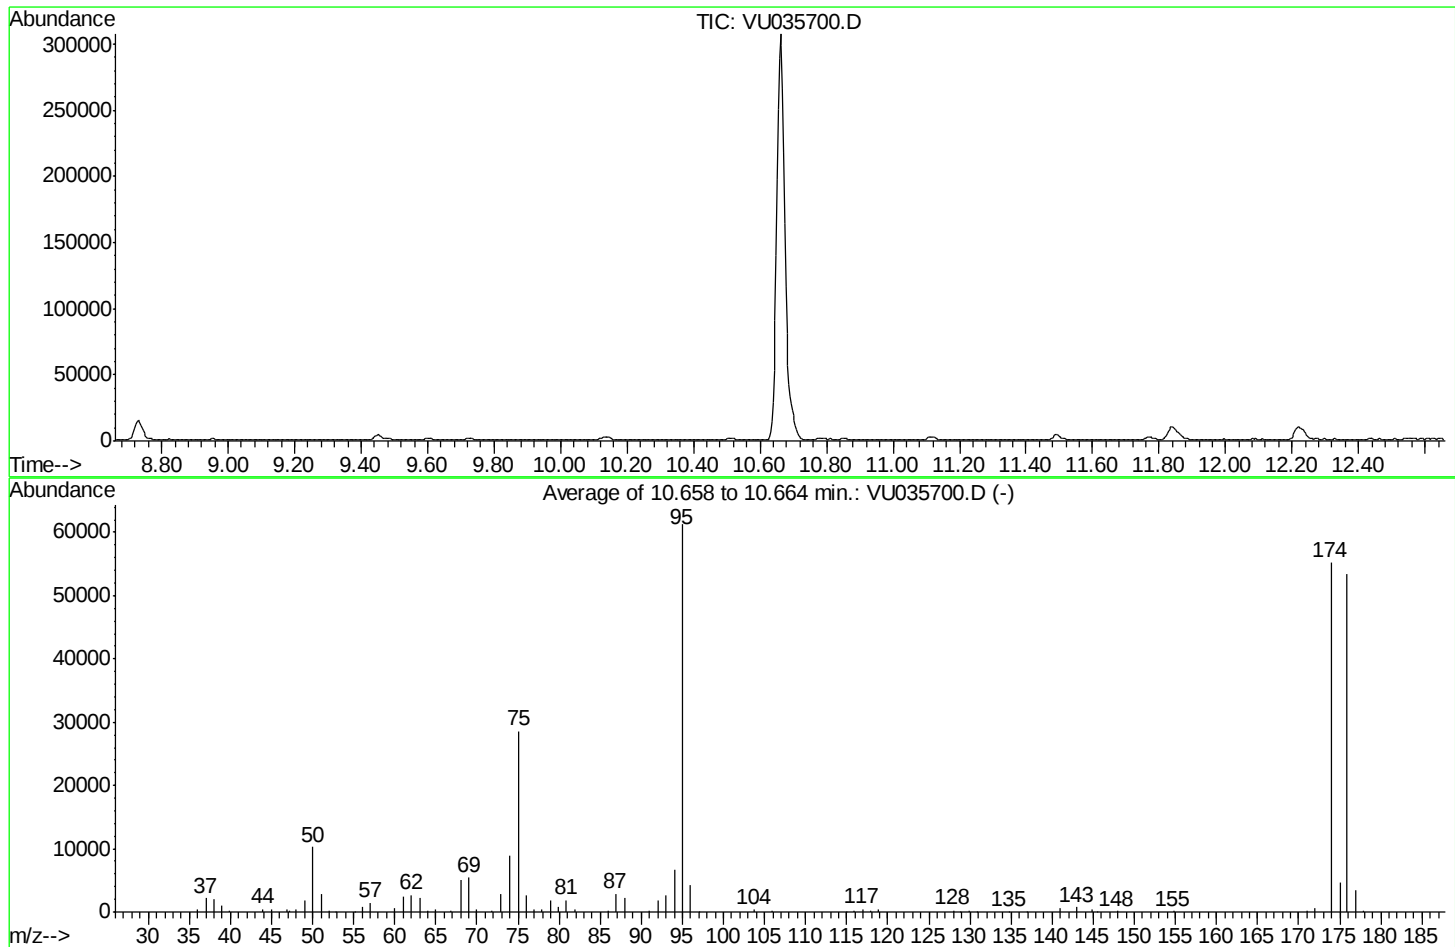

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10241	PASS
75	95	30	80	46.7	28624	PASS
95	95	100	100	100.0	61266	PASS
96	95	5	9	7.0	4264	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.0	55149	PASS
175	174	5	9	8.4	4609	PASS
176	174	95	101	96.9	53456	PASS
177	176	5	9	6.5	3497	PASS

m/z	Abundance
36.00	470.0
37.00	2217.0
38.00	1976.0
39.00	963.0
39.90	245.0
44.00	1162.0
45.00	398.0
46.90	562.0
47.90	315.0
49.00	1801.0
50.10	10174.0
51.00	2901.0
51.90	122.0
52.80	130.0
56.00	709.0
57.00	1307.0
59.90	566.0
61.00	2504.0
62.00	2754.0
63.10	2209.0
64.00	314.0
64.90	492.0
66.80	157.0
68.00	5160.0
69.00	5196.0
70.00	449.0
71.80	272.0
72.90	2490.0
74.00	8686.0
75.10	28112.0
76.00	2463.0
77.00	432.0
77.90	353.0
78.90	1844.0
79.90	683.0
80.90	1784.0
82.00	385.0
85.90	160.0
86.90	2872.0
88.00	2222.0
91.00	221.0
92.00	1752.0
93.00	2506.0
94.00	6701.0
95.00	59816.0
96.00	4346.0
103.80	339.0
105.90	159.0
115.80	199.0
116.90	406.0
117.90	170.0
118.90	336.0
128.00	199.0
129.90	162.0
136.90	132.0
140.90	545.0
143.00	753.0
144.90	392.0
147.90	140.0
154.80	156.0
171.00	177.0
172.00	679.0
173.90	52376.0
175.00	4404.0
175.90	50992.0
176.90	3371.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	424.0
37.00	2247.0
38.00	2107.0
39.00	936.0
39.90	258.0
40.20	218.0
44.00	1181.0
45.00	392.0
46.90	496.0
47.90	356.0
49.00	1908.0
50.00	10608.0
51.00	2889.0
52.00	162.0
52.90	100.0
55.10	120.0
56.00	808.0
57.00	1486.0
59.90	619.0
61.00	2434.0
62.00	2742.0
63.00	2260.0
64.00	297.0
64.90	500.0
66.80	141.0
68.00	5296.0
69.00	5598.0
70.00	491.0
71.80	280.0
73.00	2932.0
74.00	9249.0
75.10	29448.0
76.00	2627.0
76.90	478.0
77.90	372.0
78.90	1900.0
79.90	733.0
80.90	1916.0
81.90	456.0
86.00	137.0
86.90	2917.0
87.90	2200.0
91.00	243.0
92.00	1812.0
93.00	2714.0
94.00	6799.0
95.00	63096.0
96.00	4374.0
103.80	319.0
105.80	187.0
115.80	218.0
117.00	450.0
117.90	204.0
118.90	352.0
128.00	222.0
129.90	136.0
130.90	131.0
134.80	105.0
140.90	621.0
143.00	822.0
144.80	358.0
147.90	133.0
154.80	133.0
170.90	193.0
172.00	685.0
173.90	56808.0
175.00	4802.0
175.90	55224.0
177.00	3569.0
177.90	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	333.0
37.00	2118.0
38.00	1944.0
39.00	879.0
39.90	219.0
40.20	206.0
44.00	1153.0
44.90	419.0
46.90	480.0
47.20	446.0
47.90	349.0
49.00	1839.0
50.00	9941.0
51.00	2740.0
52.00	140.0
55.10	144.0
56.00	770.0
57.00	1482.0
59.90	628.0
61.00	2208.0
62.00	2480.0
63.00	2008.0
64.00	254.0
65.00	438.0
66.90	112.0
68.00	5004.0
69.00	5500.0
70.00	453.0
71.90	267.0
73.00	3013.0
74.00	9033.0
75.10	28312.0
76.00	2554.0
76.90	491.0
77.90	323.0
78.90	1914.0
79.90	735.0
80.90	1885.0
81.90	551.0
86.10	160.0
86.90	2800.0
87.90	2189.0
91.00	204.0
92.00	1750.0
93.00	2497.0
94.00	6531.0
95.00	60888.0
96.00	4074.0
97.00	124.0
103.80	320.0
105.80	242.0
114.90	111.0
115.80	227.0
116.90	451.0
117.90	174.0
118.90	322.0
128.00	195.0
128.80	131.0
129.90	151.0
130.90	123.0
134.80	121.0
141.00	667.0
143.00	786.0
144.80	356.0
145.50	114.0
147.90	116.0
154.80	104.0
170.90	159.0
171.90	700.0
174.00	56264.0
175.00	4621.0
175.90	54152.0
177.00	3553.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Scan 2886 (10.619 min): VU035700.D
BFB26

m/z	Abundance
40.10	198.0
43.90	738.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26