




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056292.D
Acq On : 14 Nov 2023 08:36
Operator : MD/SY
Sample : 05372-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDR6

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:37:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

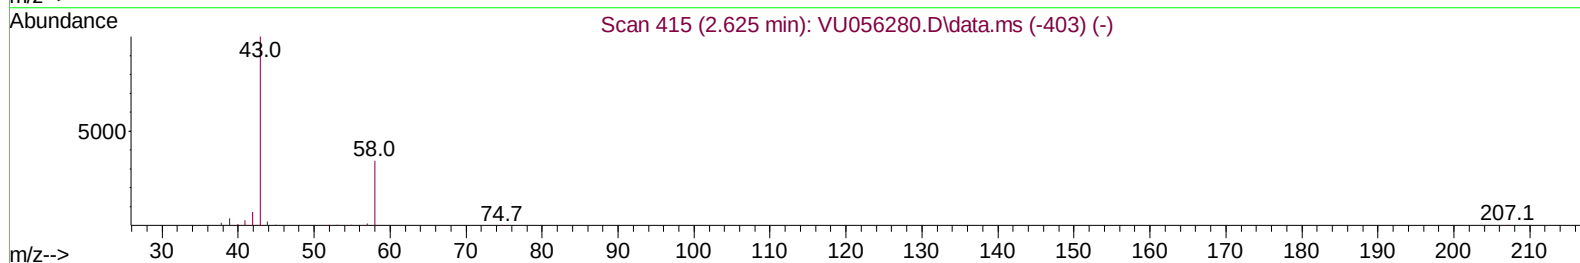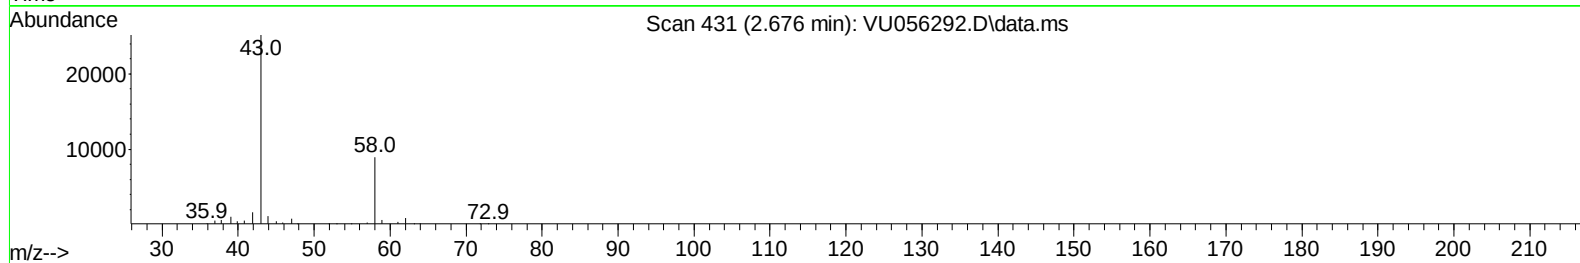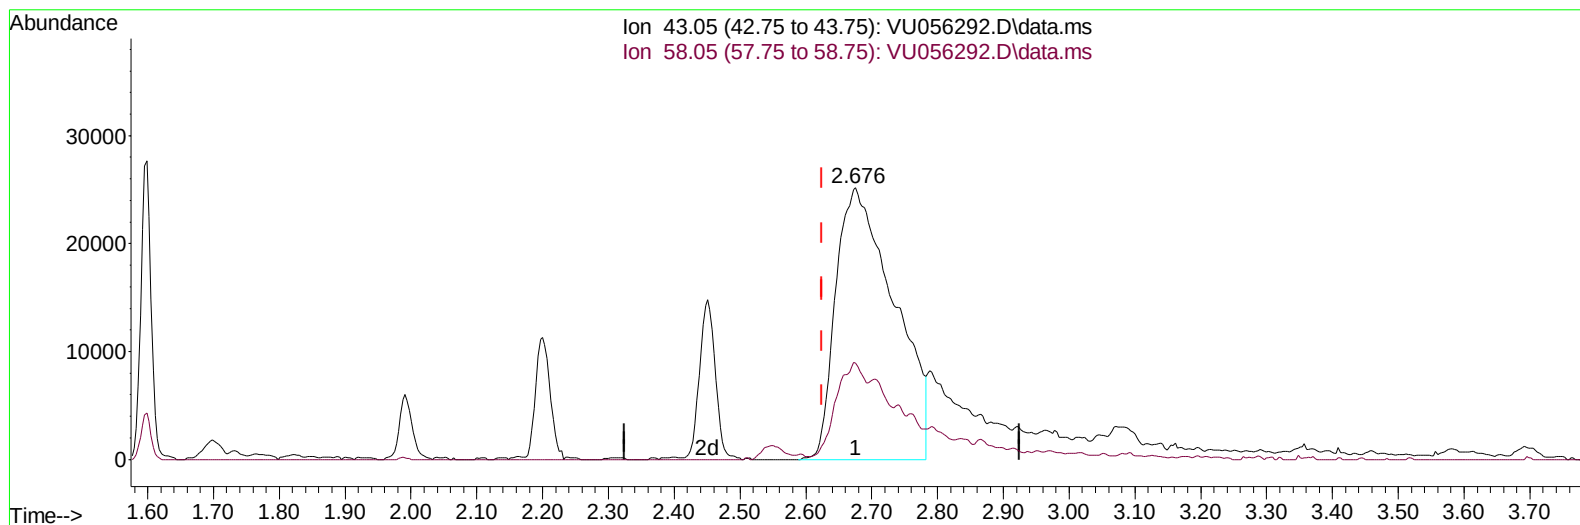

TIC: VU056292.D\data.ms

(13) Acetone (T)

2.676min (+ 0.051) 42.22 ug/L

response 154961

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.00	17.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056292.D
 Acq On : 14 Nov 2023 08:36
 Operator : MD/SY
 Sample : 05372-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDR6

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:37:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

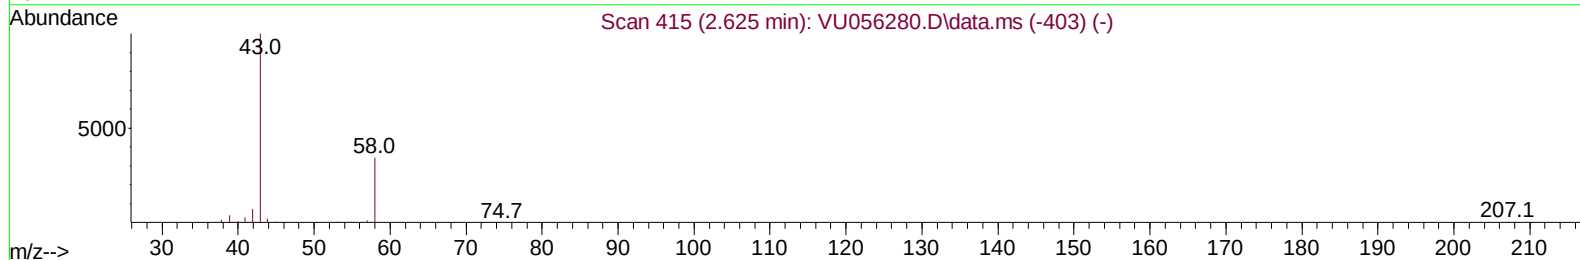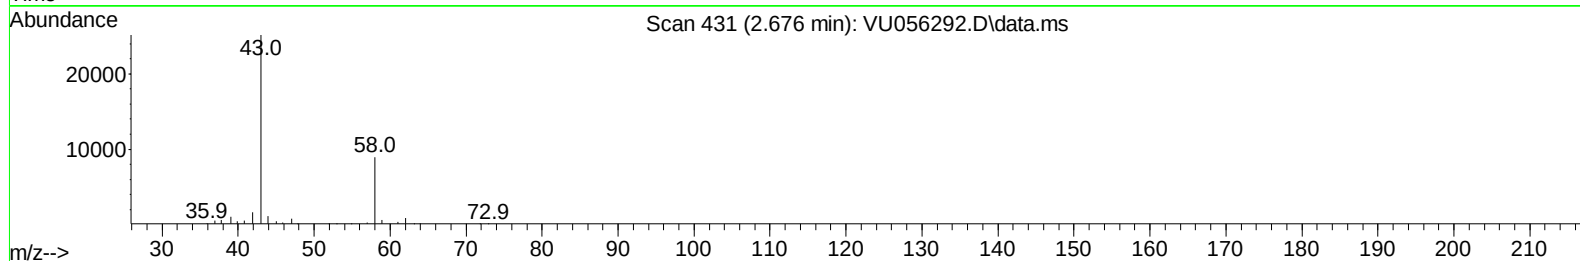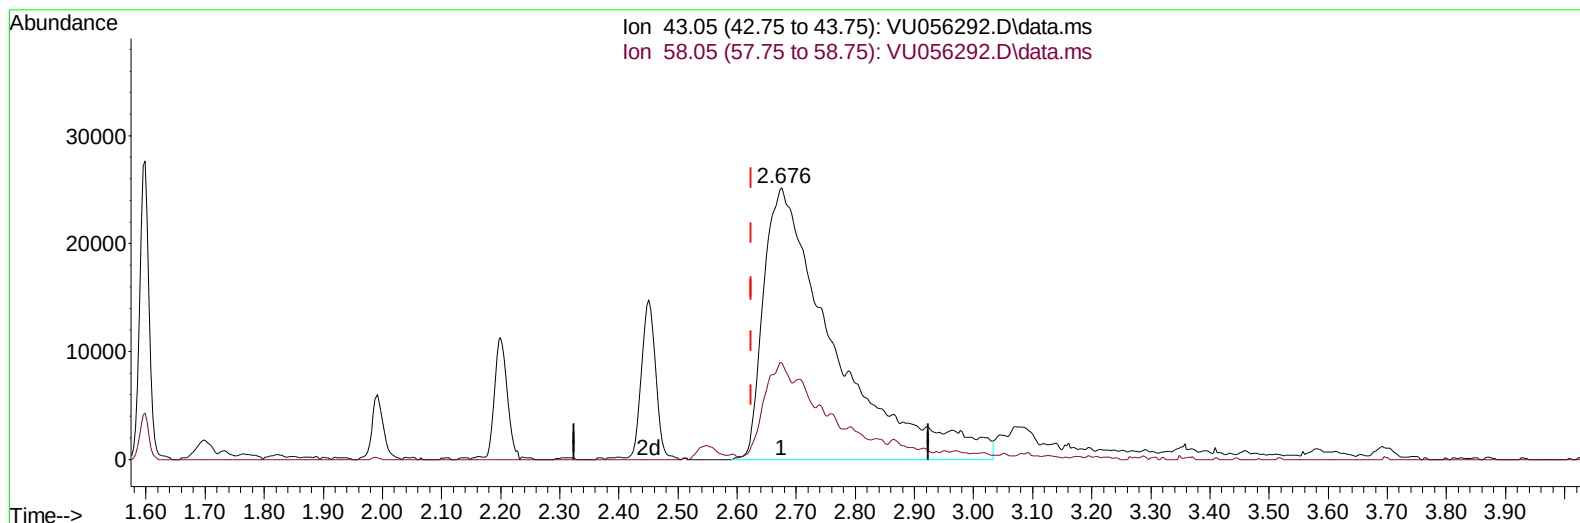

TIC: VU056292.D\data.ms

(13) Acetone (T)

2.676min (+ 0.051) 57.08 ug/L m

response 209482

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.00	12.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056292.D
Acq On : 14 Nov 2023 08:36
Operator : MD/SY
Sample : 05372-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDR6

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 15 00:37:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration

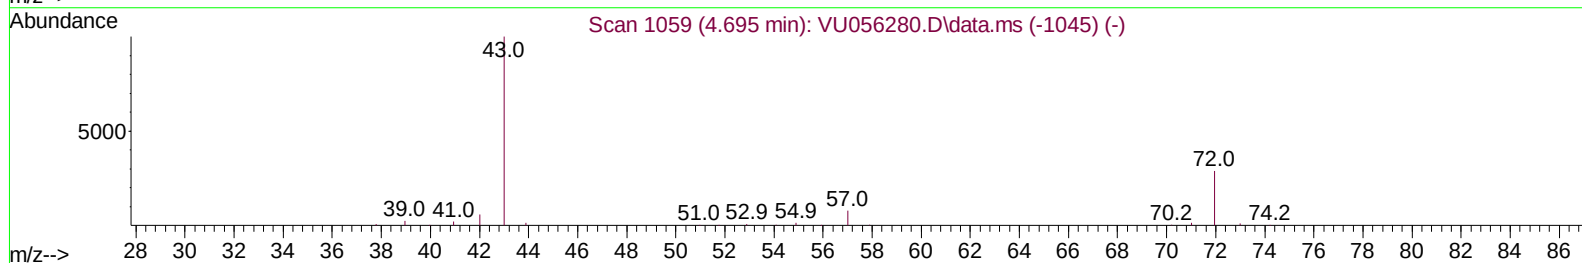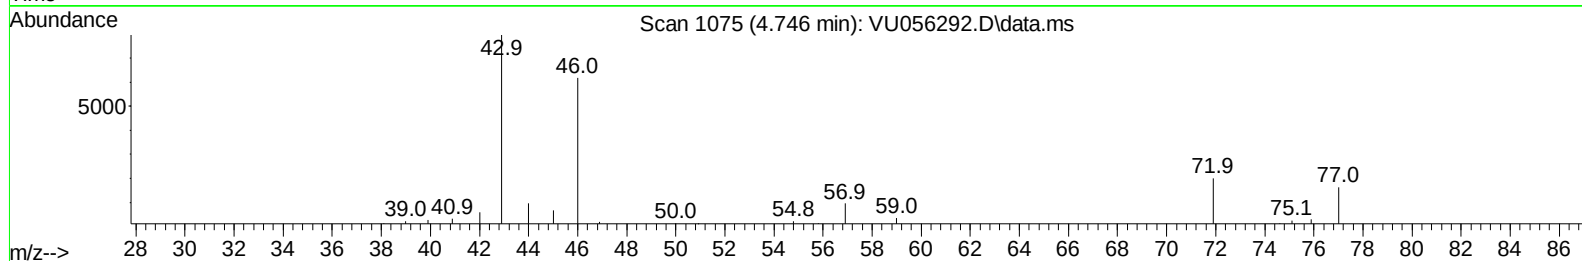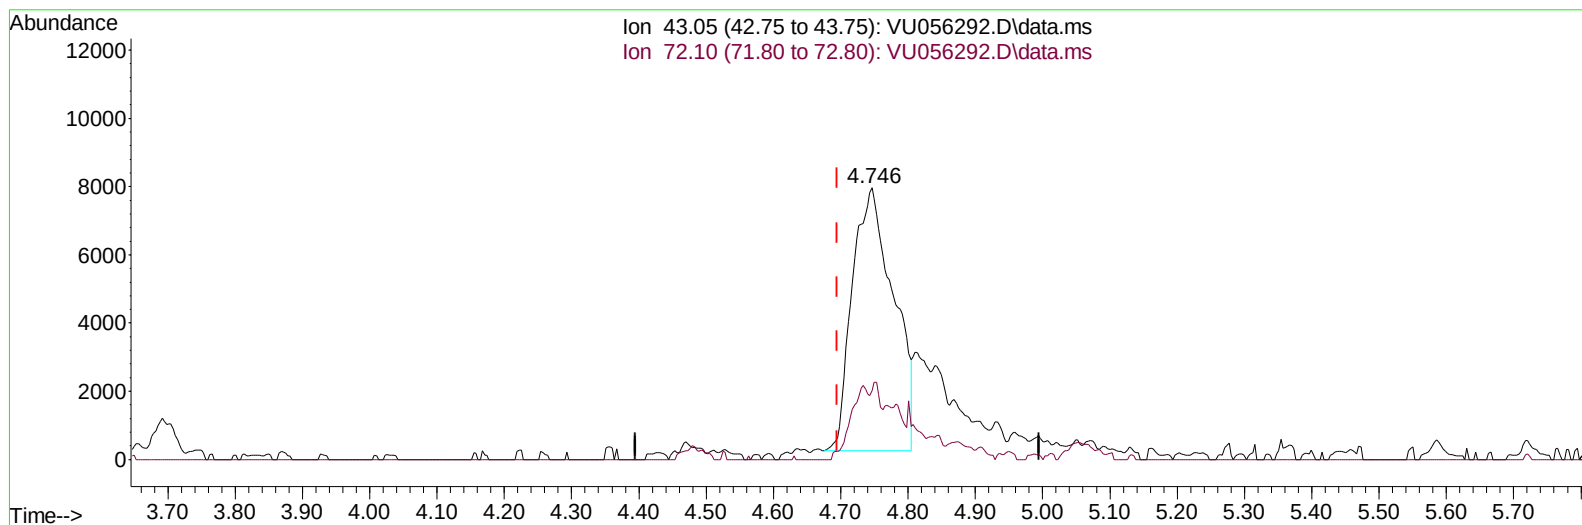

TIC: VU056292.D\data.ms

(21) 2-Butanone (T)

4.746min (+ 0.051) 6.84 ug/L

response 32565

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.40	2.19#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056292.D
 Acq On : 14 Nov 2023 08:36
 Operator : MD/SY
 Sample : 05372-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDR6

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:37:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

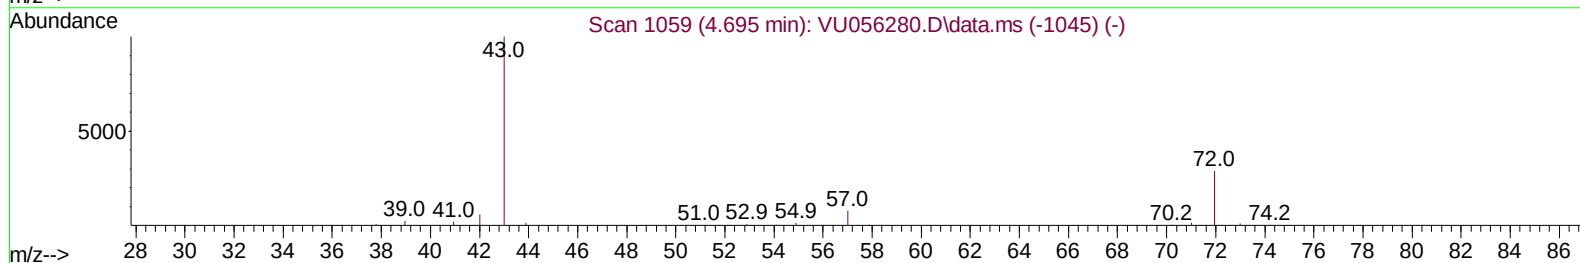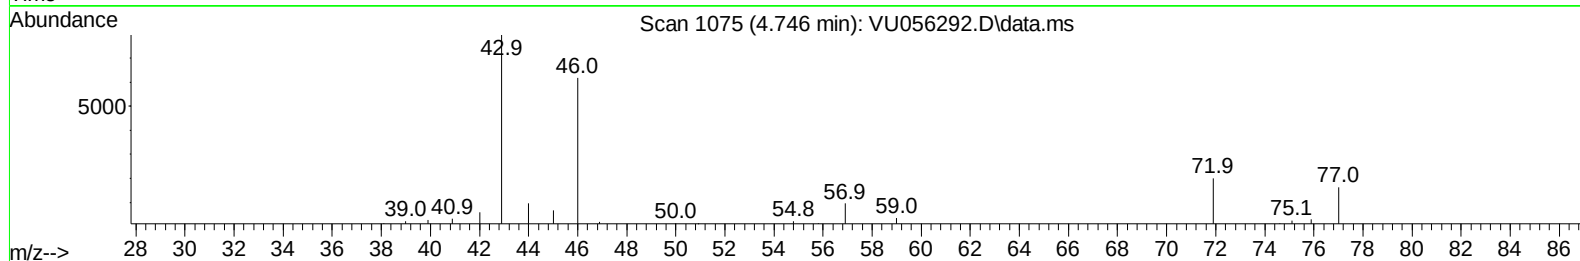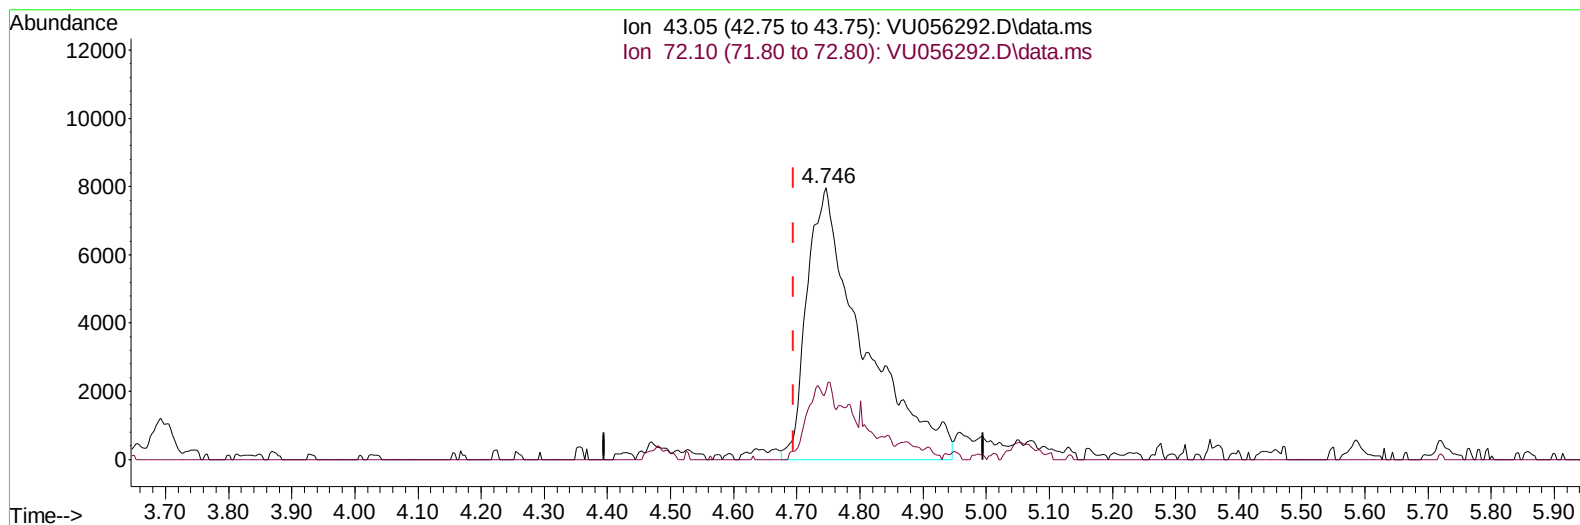

TIC: VU056292.D\data.ms

(21) 2-Butanone (T)

4.746min (+ 0.051) 10.35 ug/L m

response 49277

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.40	1.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056292.D
 Acq On : 14 Nov 2023 08:36
 Operator : MD/SY
 Sample : 05372-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDR6

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:37:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		288916	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		280668	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		127891	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		60373	2.794	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	55.800%	
7) Chloroethane-d5	1.911	69		60716	3.664	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	73.200%	
11) 1,1-Dichloroethene-d2	2.563	65		30442	3.192	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	63.800%	
20) 2-Butanone-d5	4.650	46		122614	28.455	ug/L	0.03
Spiked Amount 50.000	Range 40	- 130		Recovery	=	56.920%	
24) Chloroform-d	5.058	84		152373	3.645	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	73.000%	
26) 1,2-Dichloroethane-d4	5.698	65		71624	3.708	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	74.200%	
32) Benzene-d6	5.721	84		293878	3.514	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	70.200%	
36) 1,2-Dichloropropane-d6	6.685	67		92408	3.667	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	73.400%	
41) Toluene-d8	7.894	98		249907	3.384	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	67.600%#	
43) trans-1,3-Dichloroprop...	8.174	79		30836	3.190	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	63.800%	
46) 2-Hexanone-d5	8.634	63		117026	30.809	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	61.620%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		67636	3.756	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	75.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152		89025	3.768	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	75.400%#	
Target Compounds							
3) Chloromethane	1.515	50		6871	0.294	ug/L	99
13) Acetone	2.676	43		209482m	57.079	ug/L	
21) 2-Butanone	4.746	43		49277m	10.347	ug/L	
33) Benzene	5.772	78		13186	0.165	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056292.D
Acq On : 14 Nov 2023 08:36
Operator : MD/SY
Sample : 05372-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDR6

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:37:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

