




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056293.D
Acq On : 14 Nov 2023 09:00
Operator : MD/SY
Sample : 05371-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDN5

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 15 00:38:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration

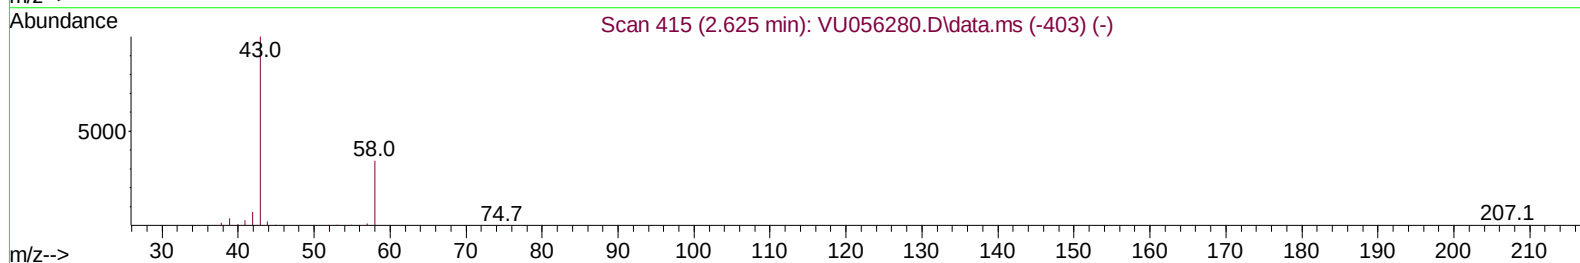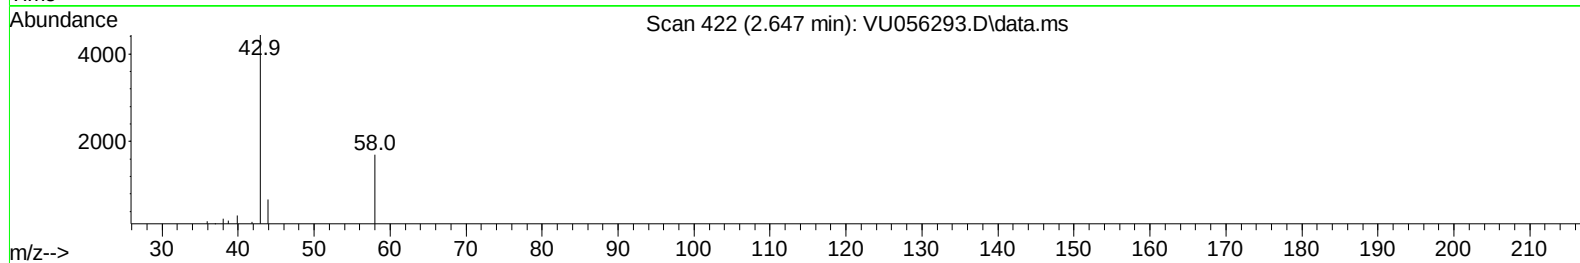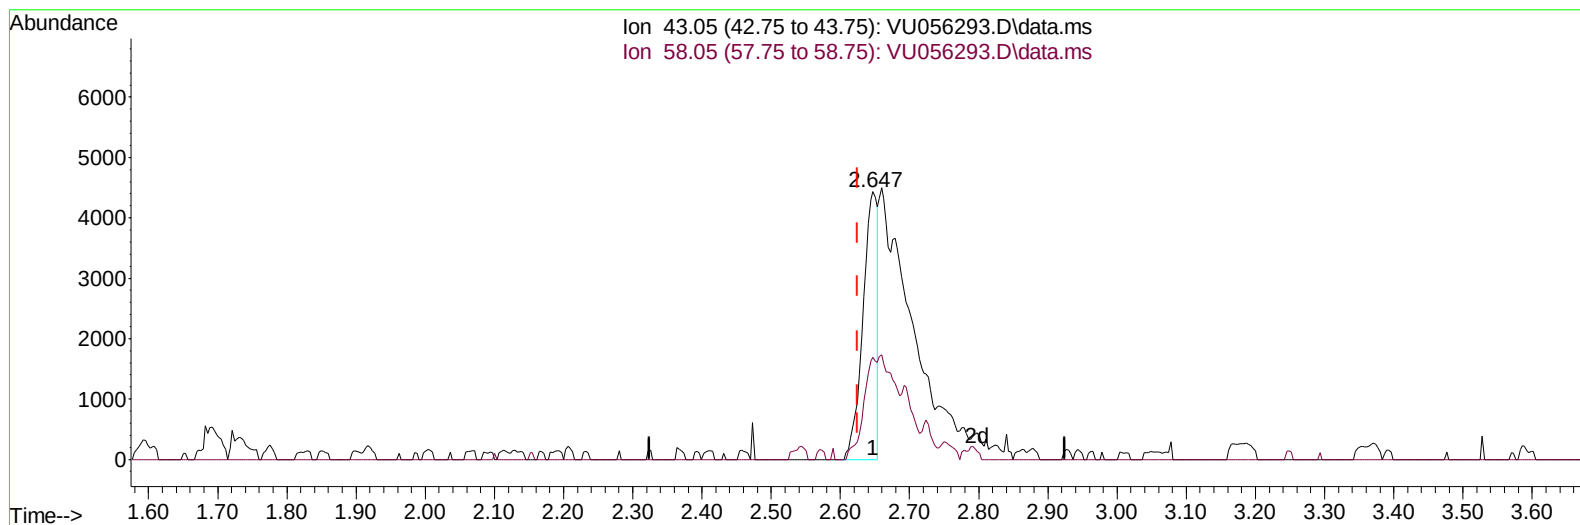

TIC: VU056293.D\data.ms

(13) Acetone (T)

2.647min (+ 0.022) 1.73 ug/L

response 6463

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.00	36.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056293.D
 Acq On : 14 Nov 2023 09:00
 Operator : MD/SY
 Sample : 05371-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDN5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

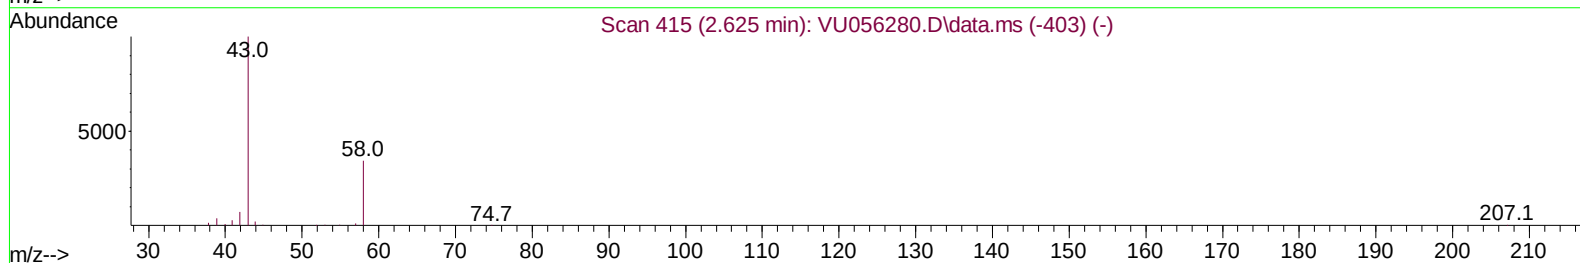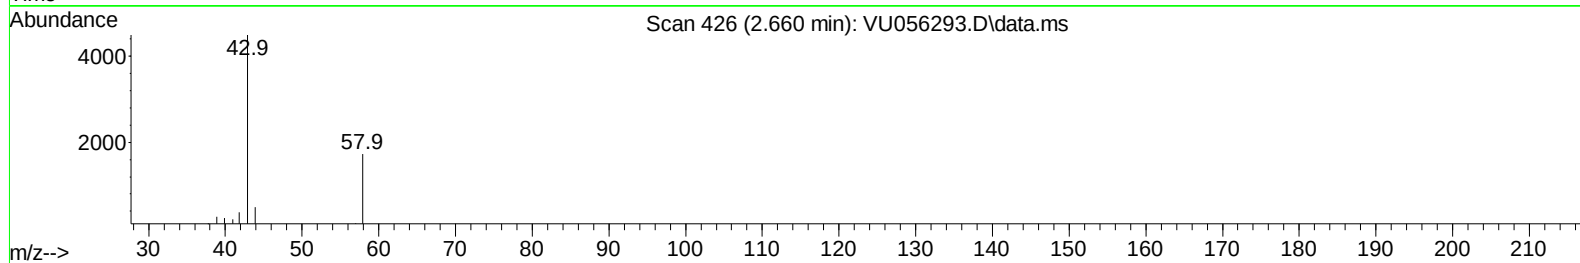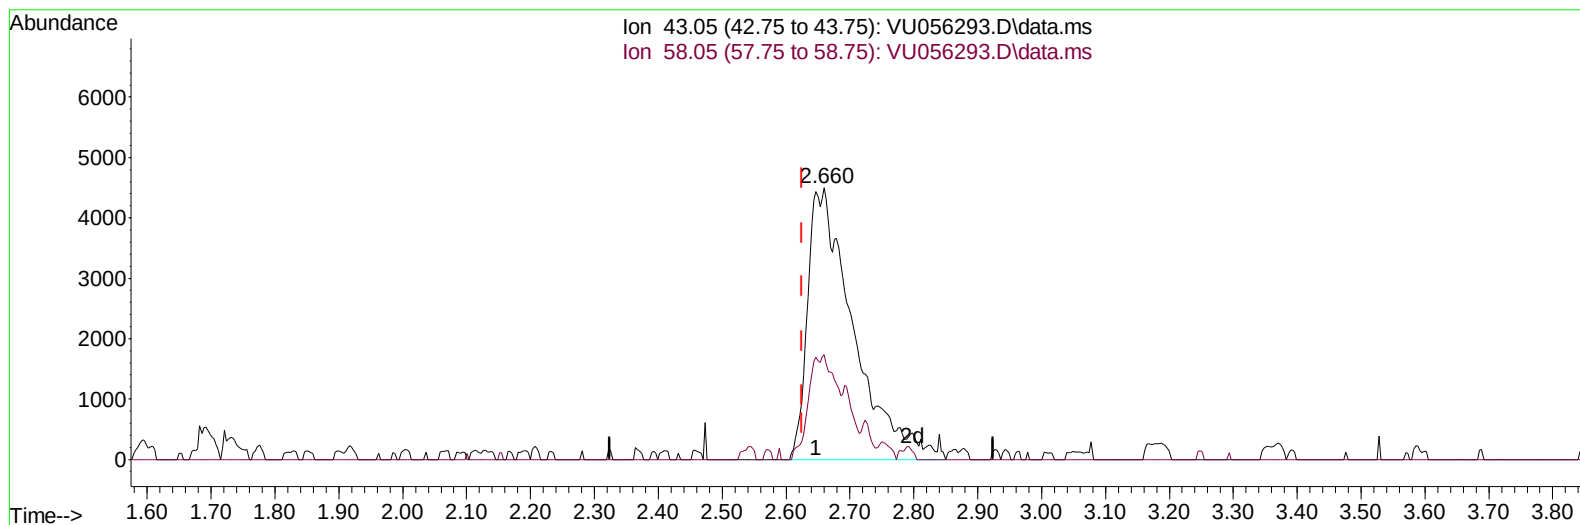

TIC: VU056293.D\data.ms

(13) Acetone (T)

2.660min (+ 0.035) 5.99 ug/L m

response 22367

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.00	10.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056293.D
 Acq On : 14 Nov 2023 09:00
 Operator : MD/SY
 Sample : 05371-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDN5

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 15 00:38:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		293768	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		296232	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		131255	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		61849	2.815	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	56.200%	
7) Chloroethane-d5	1.911	69		61264	3.636	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	72.800%	
11) 1,1-Dichloroethene-d2	2.563	65		32974	3.400	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	68.000%	
20) 2-Butanone-d5	4.637	46		172850	39.451	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery	=	78.900%	
24) Chloroform-d	5.058	84		153206	3.605	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	72.000%	
26) 1,2-Dichloroethane-d4	5.698	65		74180	3.777	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	75.600%	
32) Benzene-d6	5.721	84		292174	3.310	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	66.200%#	
36) 1,2-Dichloropropane-d6	6.685	67		91108	3.425	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	68.600%	
41) Toluene-d8	7.894	98		252484	3.240	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	64.800%#	
43) trans-1,3-Dichloroprop...	8.177	79		31564	3.094	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	61.800%	
46) 2-Hexanone-d5	8.631	63		137690	34.344	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	68.680%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		67505	3.552	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	71.000%	
66) 1,2-Dichlorobenzene-d4	12.187	152		90843	3.746	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	75.000%#	
Target Compounds						Qvalue	
12) 1,1-Dichloroethene	2.576	96		5606	0.312	ug/L #	1
13) Acetone	2.660	43		22367m	5.994	ug/L	
34) Trichloroethene	6.537	95		11542	0.501	ug/L	95
47) Tetrachloroethene	8.547	164		85713	5.519	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056293.D
Acq On : 14 Nov 2023 09:00
Operator : MD/SY
Sample : 05371-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDN5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

