

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
 Data File : VU056290.D
 Acq On : 14 Nov 2023 07:47
 Operator : MD/SY
 Sample : 05372-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDR4

Quant Time: Nov 15 00:37:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 00:09:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	295912	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	301630	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	128810	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	61877	2.796	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	56.000%
7) Chloroethane-d5	1.911	69	53691	3.164	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	63.200%#
11) 1,1-Dichloroethene-d2	2.563	65	33372	3.417	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.400%
20) 2-Butanone-d5	4.621	46	170319	38.591	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.180%
24) Chloroform-d	5.058	84	152296	3.557	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.200%
26) 1,2-Dichloroethane-d4	5.698	65	72310	3.655	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%
32) Benzene-d6	5.724	84	286551	3.189	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	63.800%#
36) 1,2-Dichloropropane-d6	6.685	67	90750	3.351	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	67.000%
41) Toluene-d8	7.894	98	250066	3.151	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.000%#
43) trans-1,3-Dichloroprop...	8.177	79	29973	2.885	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.800%
46) 2-Hexanone-d5	8.631	63	136779	33.506	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.020%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	67993	3.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	70.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	89002	3.740	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.800%#
Target Compounds						
					Qvalue	
3) Chloromethane	1.518	50	6058	0.253	ug/L	97
13) Acetone	2.628	43	179538	47.763	ug/L	100
19) 1,1-Dichloroethane	3.866	63	7968	0.216	ug/L	96
21) 2-Butanone	4.711	43	47835	9.807	ug/L	92
22) cis-1,2-Dichloroethene	4.663	96	10636	0.503	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056290.D
Acq On : 14 Nov 2023 07:47
Operator : MD/SY
Sample : 05372-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDR4

Quant Time: Nov 15 00:37:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 00:09:07 2023
Response via : Initial Calibration




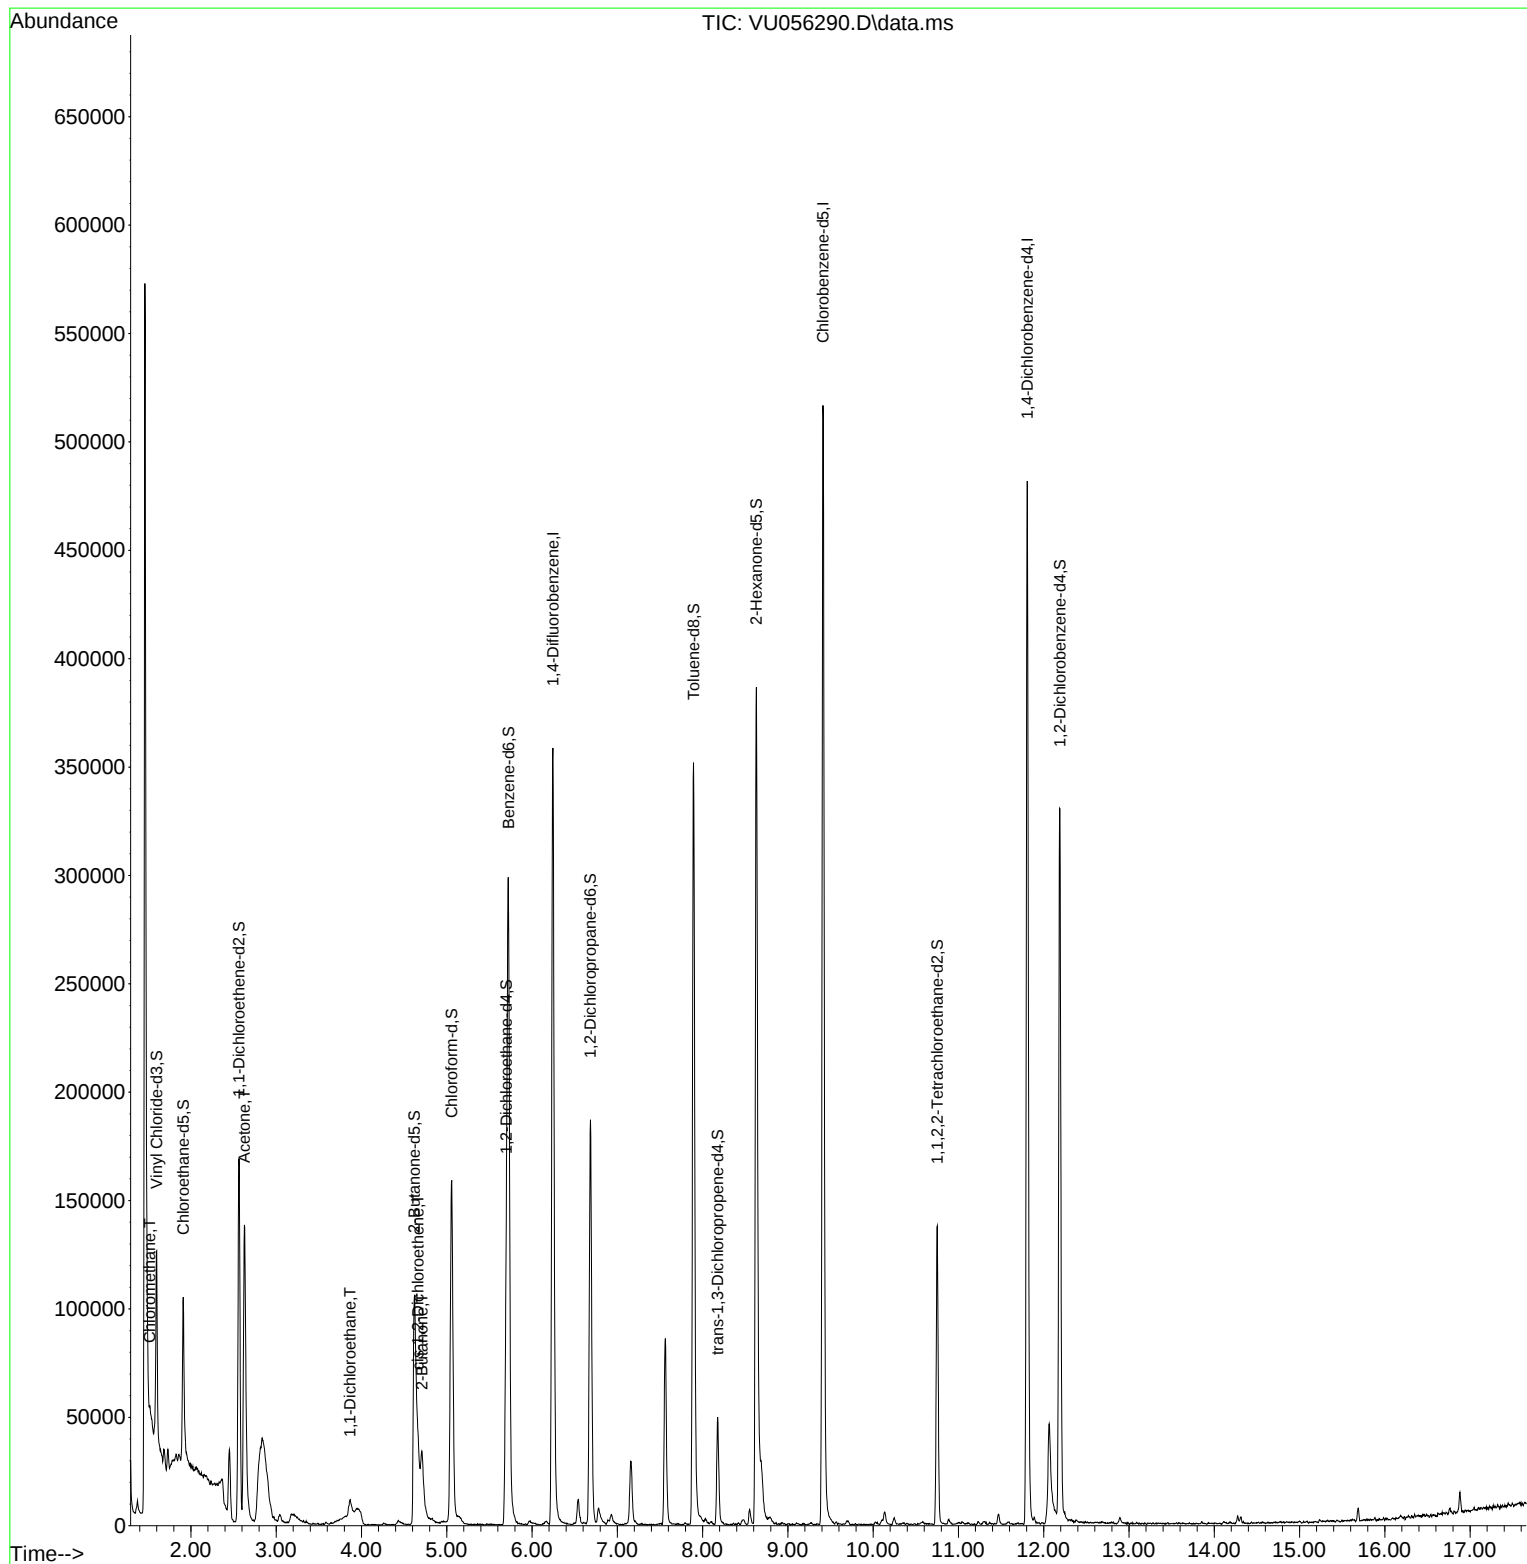


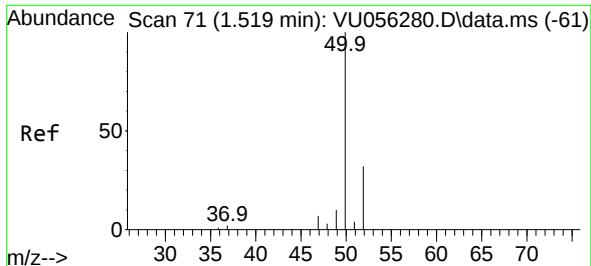

#3
Chloromethane
Concen: 0.253 ug/L
RT: 1.518 min Scan# 71
Delta R.T. -0.000 min
Lab File: VU056290.D
Acq: 14 Nov 2023 07:47




Instrument :
MSVOA_U
ClientSampleId :
GCDR4


Tgt Ion: 50 Resp: 6058
Ion Ratio Lower Upper
50 100
52 36.6 24.3 45.1

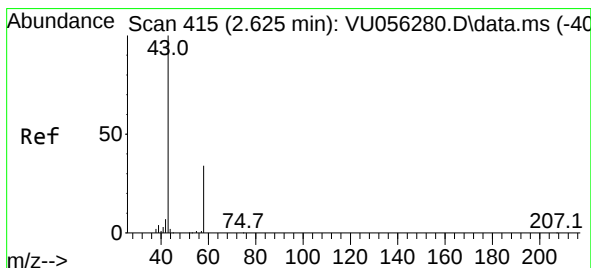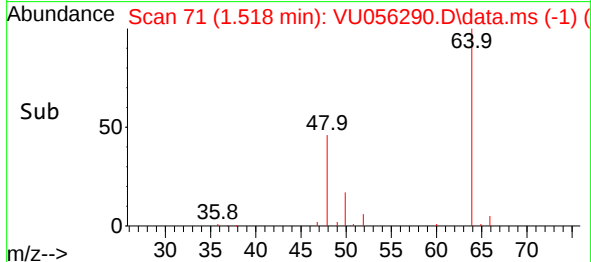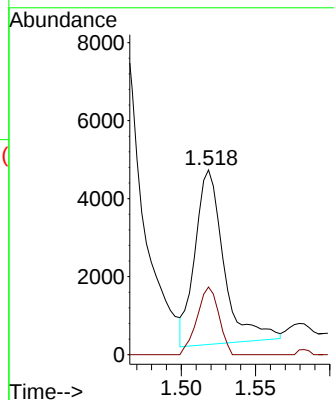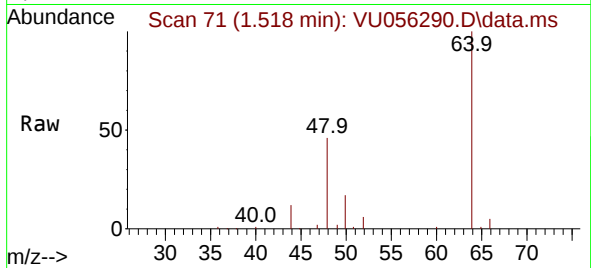

#13
Acetone
Concen: 47.763 ug/L
RT: 2.628 min Scan# 416
Delta R.T. 0.003 min
Lab File: VU056290.D
Acq: 14 Nov 2023 07:47

Tgt Ion: 43 Resp: 179538
Ion Ratio Lower Upper
43 100
58 34.8 0.0 70.0

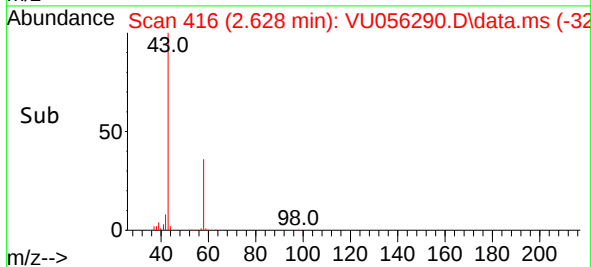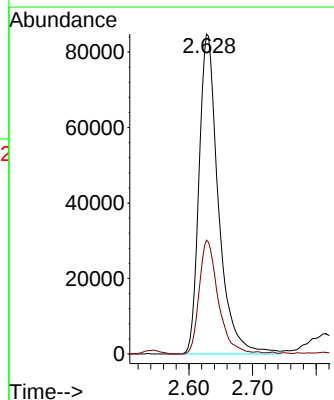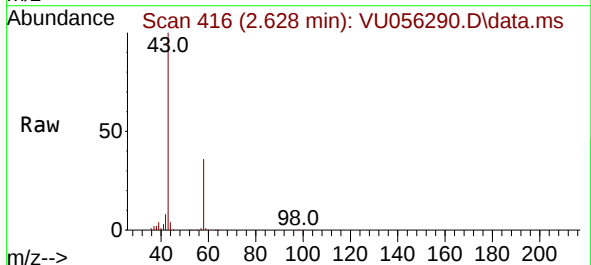

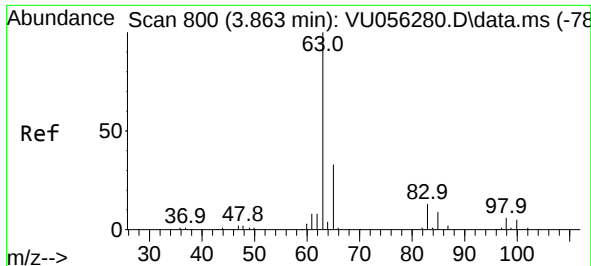

#19

1,1-Dichloroethane

Concen: 0.216 ug/L

RT: 3.866 min Scan# 800

Delta R.T. 0.003 min

Lab File: VU056290.D

Acq: 14 Nov 2023 07:47

Instrument :

MSVOA_U

ClientSampleId :

GCDR4





Tgt Ion: 63 Resp: 7968

Ion Ratio Lower Upper

63 100

65 27.8 21.8 40.6

83 13.8 9.7 17.9

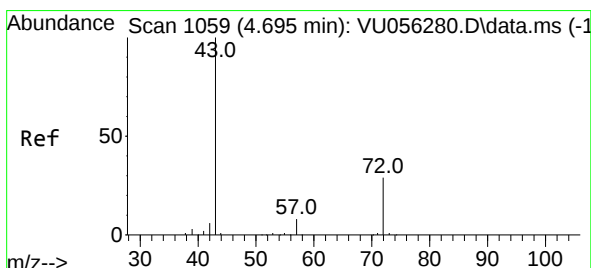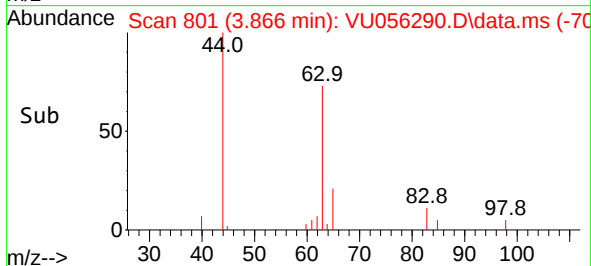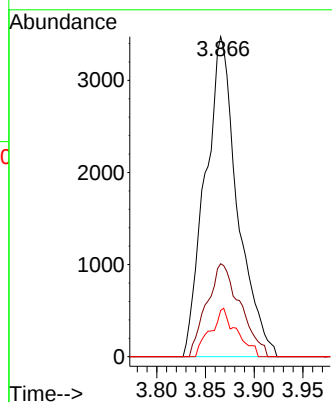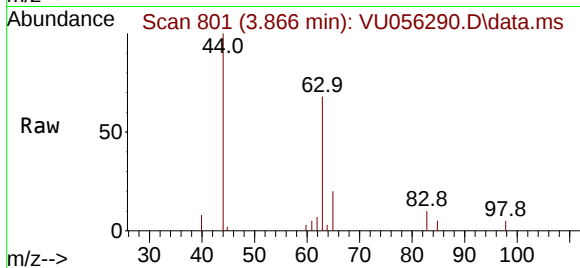

#21

2-Butanone

Concen: 9.807 ug/L

RT: 4.711 min Scan# 1064

Delta R.T. 0.016 min

Lab File: VU056290.D




Acq: 14 Nov 2023 07:47


Tgt Ion: 43 Resp: 47835

Ion Ratio Lower Upper

43 100

72 32.8 14.2 42.6

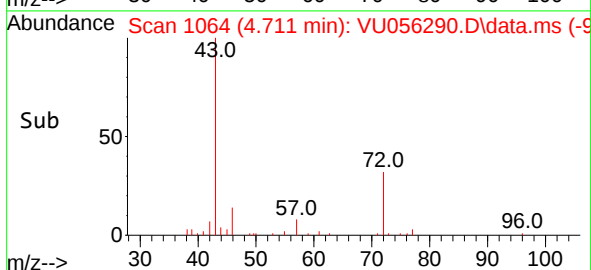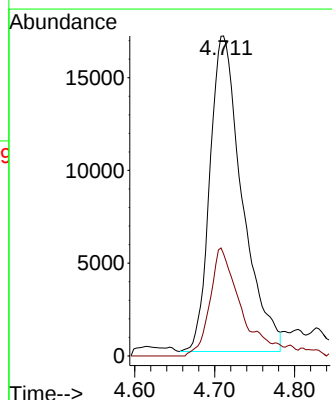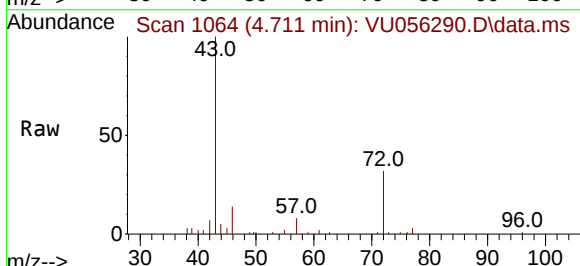

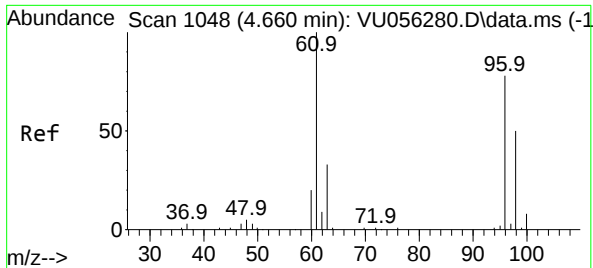

#22
 cis-1,2-Dichloroethene
 Concen: 0.503 ug/L
 RT: 4.663 min Scan# 1049
 Delta R.T. 0.003 min
 Lab File: VU056290.D
 Acq: 14 Nov 2023 07:47

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDR4

Tgt Ion: 96	Resp: 10636
Ion Ratio	Lower Upper
96	100
61	130.7 93.2 173.2
98	59.6 44.8 83.2

