


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111323\
Data File : VU056248.D
Acq On : 13 Nov 2023 11:40
Operator : MD/SY
Sample : BFB072
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB072

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 17 04:03:21 2023

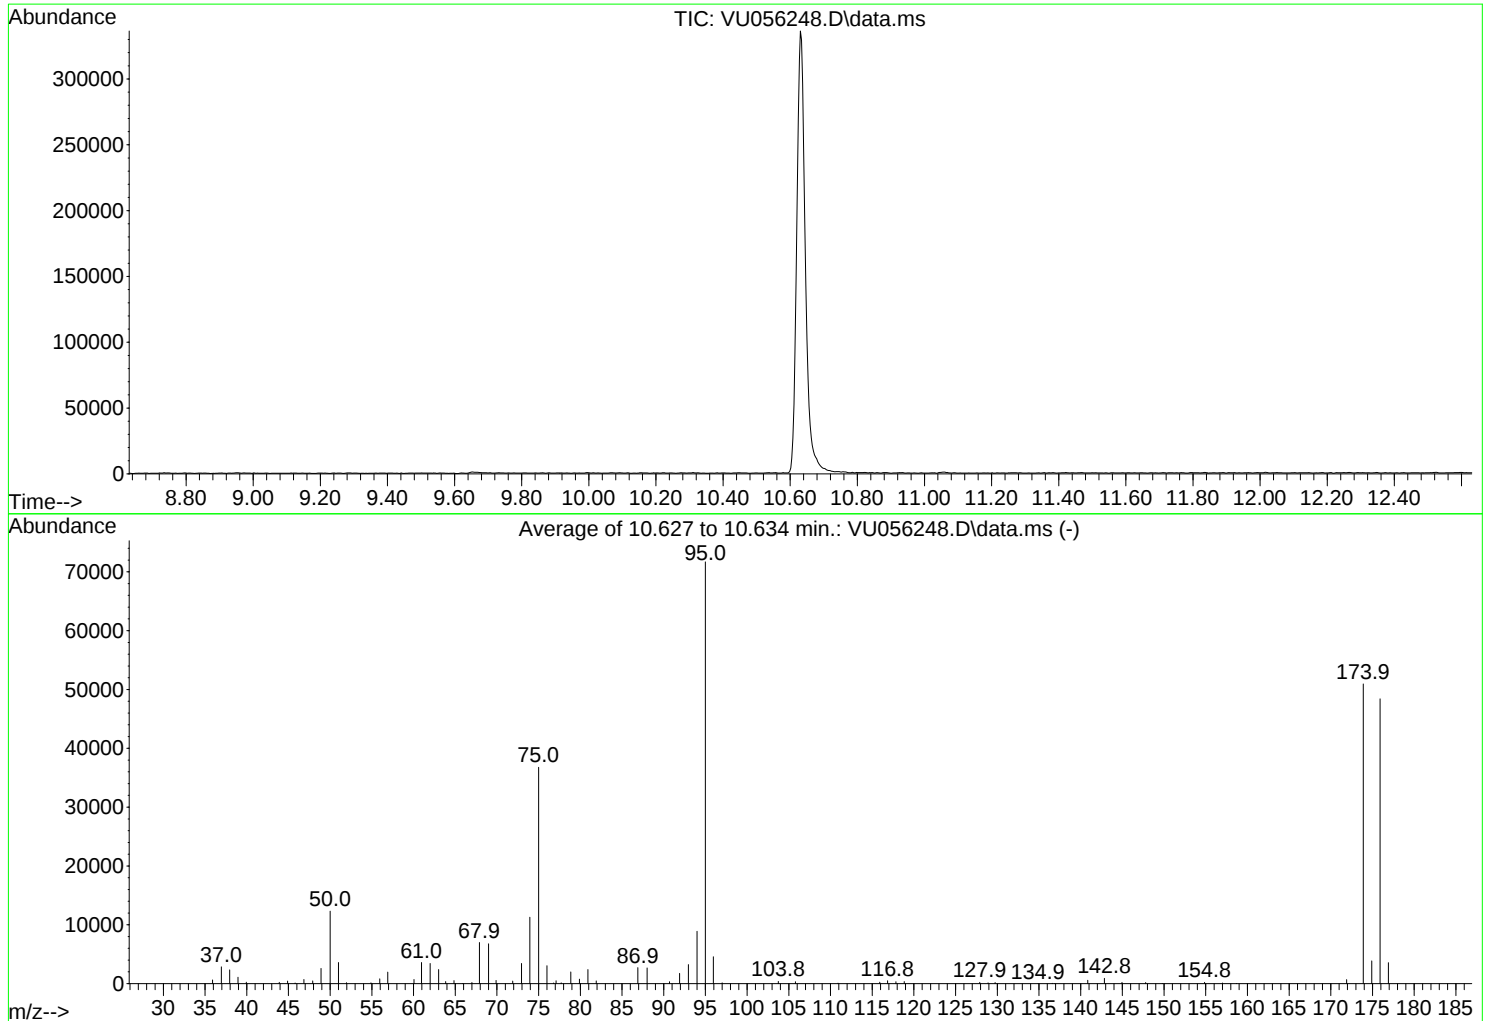

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	12333	PASS
75	95	30	80	51.3	36784	PASS
95	95	100	100	100.0	71701	PASS
96	95	5	9	6.4	4568	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.1	50949	PASS
175	174	5	9	7.6	3863	PASS
176	174	95	101	95.0	48421	PASS
177	176	5	9	7.3	3557	PASS

m/z	Abundance
39.70	163.0
43.90	604.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	553.0
37.00	2715.0
38.00	2351.0
39.00	1000.0
39.90	263.0
43.90	870.0
44.90	455.0
47.00	779.0
47.80	445.0
48.90	2374.0
50.00	12090.0
51.00	3802.0
51.90	216.0
55.00	135.0
56.00	695.0
56.90	1740.0
60.00	591.0
60.90	3387.0
62.00	3506.0
63.00	2213.0
64.00	414.0
64.80	460.0
67.00	178.0
67.90	6690.0
69.00	6176.0
69.90	506.0
71.90	387.0
73.00	3307.0
74.00	10870.0
75.00	35368.0
76.00	3057.0
77.10	518.0
78.90	1984.0
79.90	666.0
80.90	2397.0
81.90	411.0
86.90	2536.0
88.00	2834.0
90.70	412.0
91.90	1888.0
92.90	3289.0
94.00	8519.0
95.00	70200.0
96.00	4692.0
97.00	137.0
103.70	390.0
105.80	334.0
110.90	117.0
115.90	349.0
116.90	491.0
117.90	238.0
118.80	373.0
127.90	225.0
128.90	169.0
129.90	162.0
134.90	125.0
136.60	135.0
141.00	540.0
142.90	883.0
145.00	221.0
147.80	137.0
149.80	113.0
154.90	216.0
171.90	666.0
173.90	48080.0
174.90	3987.0
175.90	45384.0
176.90	3507.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	657.0
37.00	2950.0
37.90	2394.0
38.90	1079.0
39.90	231.0
43.90	863.0
44.90	427.0
45.80	148.0
46.80	717.0
47.90	492.0
48.90	2714.0
50.00	12686.0
51.00	3653.0
52.00	179.0
54.90	129.0
56.00	798.0
56.90	2053.0
60.00	753.0
61.00	3697.0
62.00	3572.0
63.00	2428.0
63.80	346.0
64.90	544.0
67.00	211.0
67.90	7213.0
69.00	6918.0
69.90	596.0
71.90	459.0
72.90	3580.0
74.00	11677.0
75.00	37888.0
76.00	3107.0
77.10	550.0
77.70	217.0
78.90	2029.0
79.90	811.0
80.90	2449.0
81.90	473.0
86.90	2813.0
88.00	2773.0
90.70	342.0
91.90	1779.0
92.90	3324.0
94.00	9146.0
95.00	73824.0
96.00	4649.0
97.00	161.0
103.80	406.0
105.80	345.0
110.90	116.0
115.90	248.0
116.80	486.0
117.80	320.0
118.80	371.0
127.90	254.0
128.90	139.0
129.70	197.0
140.80	565.0
142.80	896.0
145.00	207.0
147.80	202.0
154.90	238.0
157.00	140.0
171.90	705.0
173.90	52496.0
174.90	3963.0
175.90	49896.0
176.90	3724.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	675.0
36.90	2938.0
37.90	2286.0
38.90	1150.0
40.00	240.0
43.90	782.0
44.90	437.0
45.80	198.0
46.80	652.0
48.00	464.0
48.90	2704.0
50.00	12224.0
51.00	3323.0
52.00	133.0
54.80	144.0
55.90	940.0
56.90	2084.0
60.10	767.0
61.00	3660.0
62.00	3193.0
63.00	2517.0
63.80	345.0
64.90	547.0
65.90	110.0
67.00	220.0
67.90	7058.0
69.00	7224.0
69.90	545.0
71.90	478.0
72.90	3409.0
73.90	11358.0
75.00	37096.0
76.00	3005.0
76.80	354.0
77.10	398.0
77.70	234.0
78.80	1955.0
79.90	830.0
80.90	2369.0
81.90	525.0
86.90	2816.0
88.00	2430.0
90.70	231.0
91.90	1581.0
93.00	3141.0
94.00	8988.0
95.00	71080.0
95.90	4362.0
97.00	142.0
103.80	360.0
105.80	295.0
115.80	158.0
116.90	518.0
117.80	409.0
118.90	322.0
127.90	227.0
128.90	114.0
129.70	250.0
136.90	107.0
140.80	625.0
142.80	922.0
144.80	207.0
147.80	222.0
154.80	217.0
157.00	178.0
158.70	107.0
171.90	700.0
173.90	52272.0
174.90	3638.0
175.90	49984.0
176.90	3439.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072