

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111418\
 Data File : VU028124.D
 Acq On : 14 Nov 2018 16:37
 Operator : MD/SY
 Sample : J5948-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9C13

Quant Time: Nov 15 05:05:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 15 04:25:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	155292	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	146130	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	67125	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	55120	4.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.60%
7) Chloroethane-d5	1.68	69	44129	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.20%
11) 1,1-Dichloroethene-d2	2.28	63	78248	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	4.19	46	182167	48.74	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.48%
24) Chloroform-d	4.65	84	91279	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.31	65	52403	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.34	84	191885	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.33	67	70119	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.57	98	168956	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
43) trans-1,3-Dichloropropene-	7.85	79	22376	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.31	63	144171	47.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.32%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	48108	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	58645	4.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	5413	2.150 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111418\
Data File : VU028124.D
Acq On : 14 Nov 2018 16:37
Operator : MD/SY
Sample : J5948-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9C13

Quant Time: Nov 15 05:05:54 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 15 04:25:02 2018
Response via : Initial Calibration

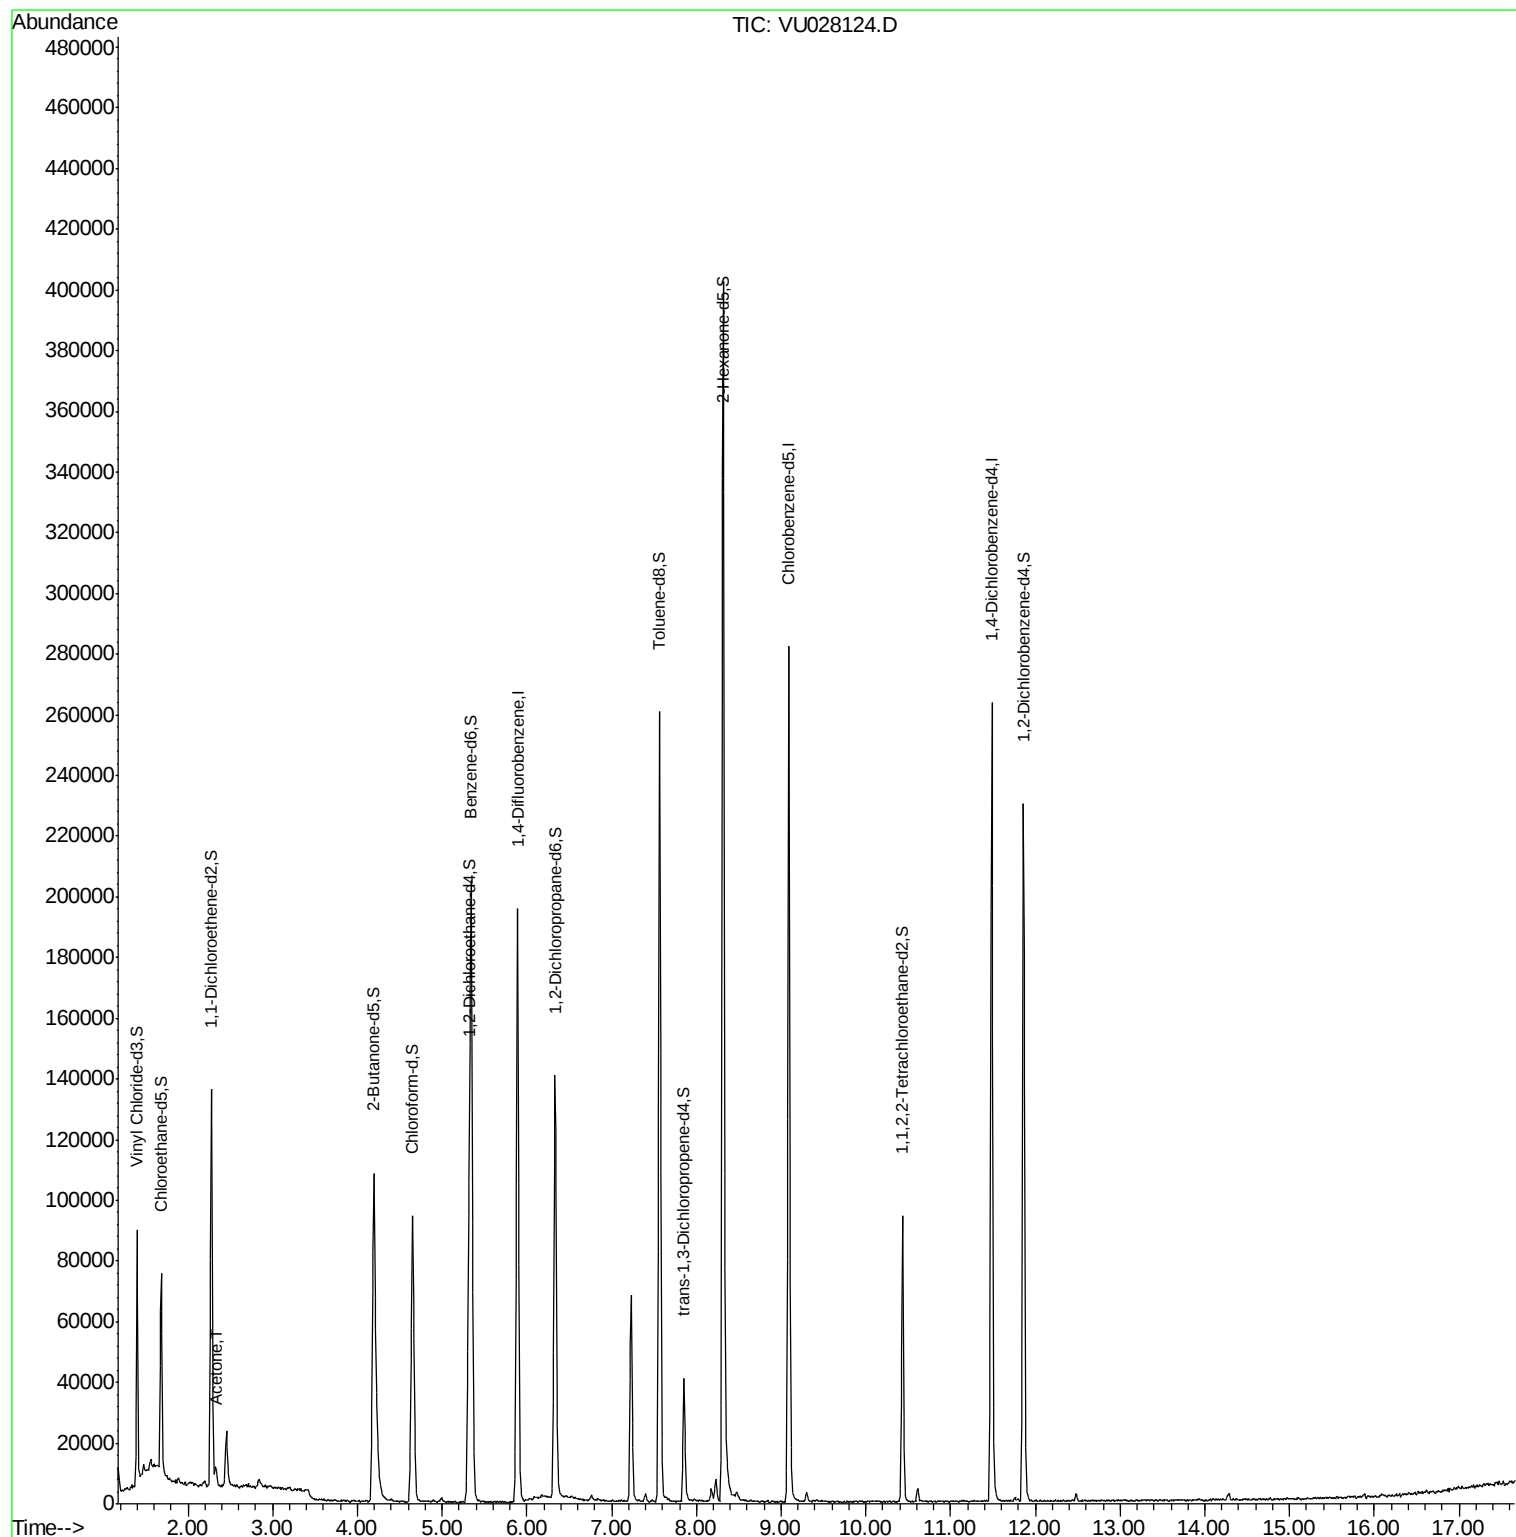

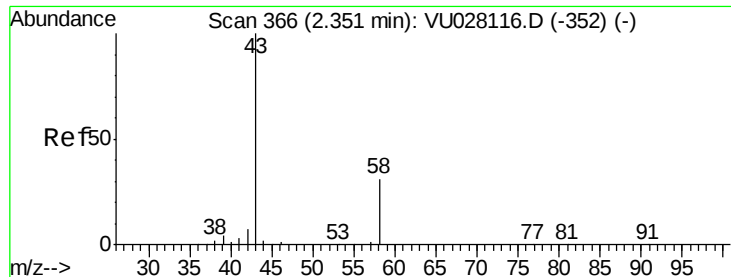

#13

Acetone

Concen: 2.150 ug/L

RT: 2.32 min Scan# 358

Delta R.T. -0.03 min

Lab File: VU028124.D

Acq: 14 Nov 2018 16:37

Instrument :
MSVOA_U
ClientSampleId :
F9C13

Tot Ion: 43 Resp: 5413

Ion Ratio Lower Upper

43 100

58 29.8 0.0 61.6

