

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111418\
 Data File : VU028133.D
 Acq On : 14 Nov 2018 20:10
 Operator : MD/SY
 Sample : J5948-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9C31

Quant Time: Nov 15 05:58:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 15 04:25:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	135573	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	126827	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	58338	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	50670	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.68	69	42140	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.40%
11) 1,1-Dichloroethene-d2	2.28	63	72021	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	4.19	46	171398	52.53	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.06%
24) Chloroform-d	4.65	84	86567	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.31	65	49722	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.34	84	178588	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.33	67	65360	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.57	98	159091	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloropropene-	7.85	79	20090	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.31	63	135042	50.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.78%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	43255	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	53581	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.33	43	2756	1.254 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111418\
Data File : VU028133.D
Acq On : 14 Nov 2018 20:10
Operator : MD/SY
Sample : J5948-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9C31

Quant Time: Nov 15 05:58:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 15 04:25:02 2018
Response via : Initial Calibration

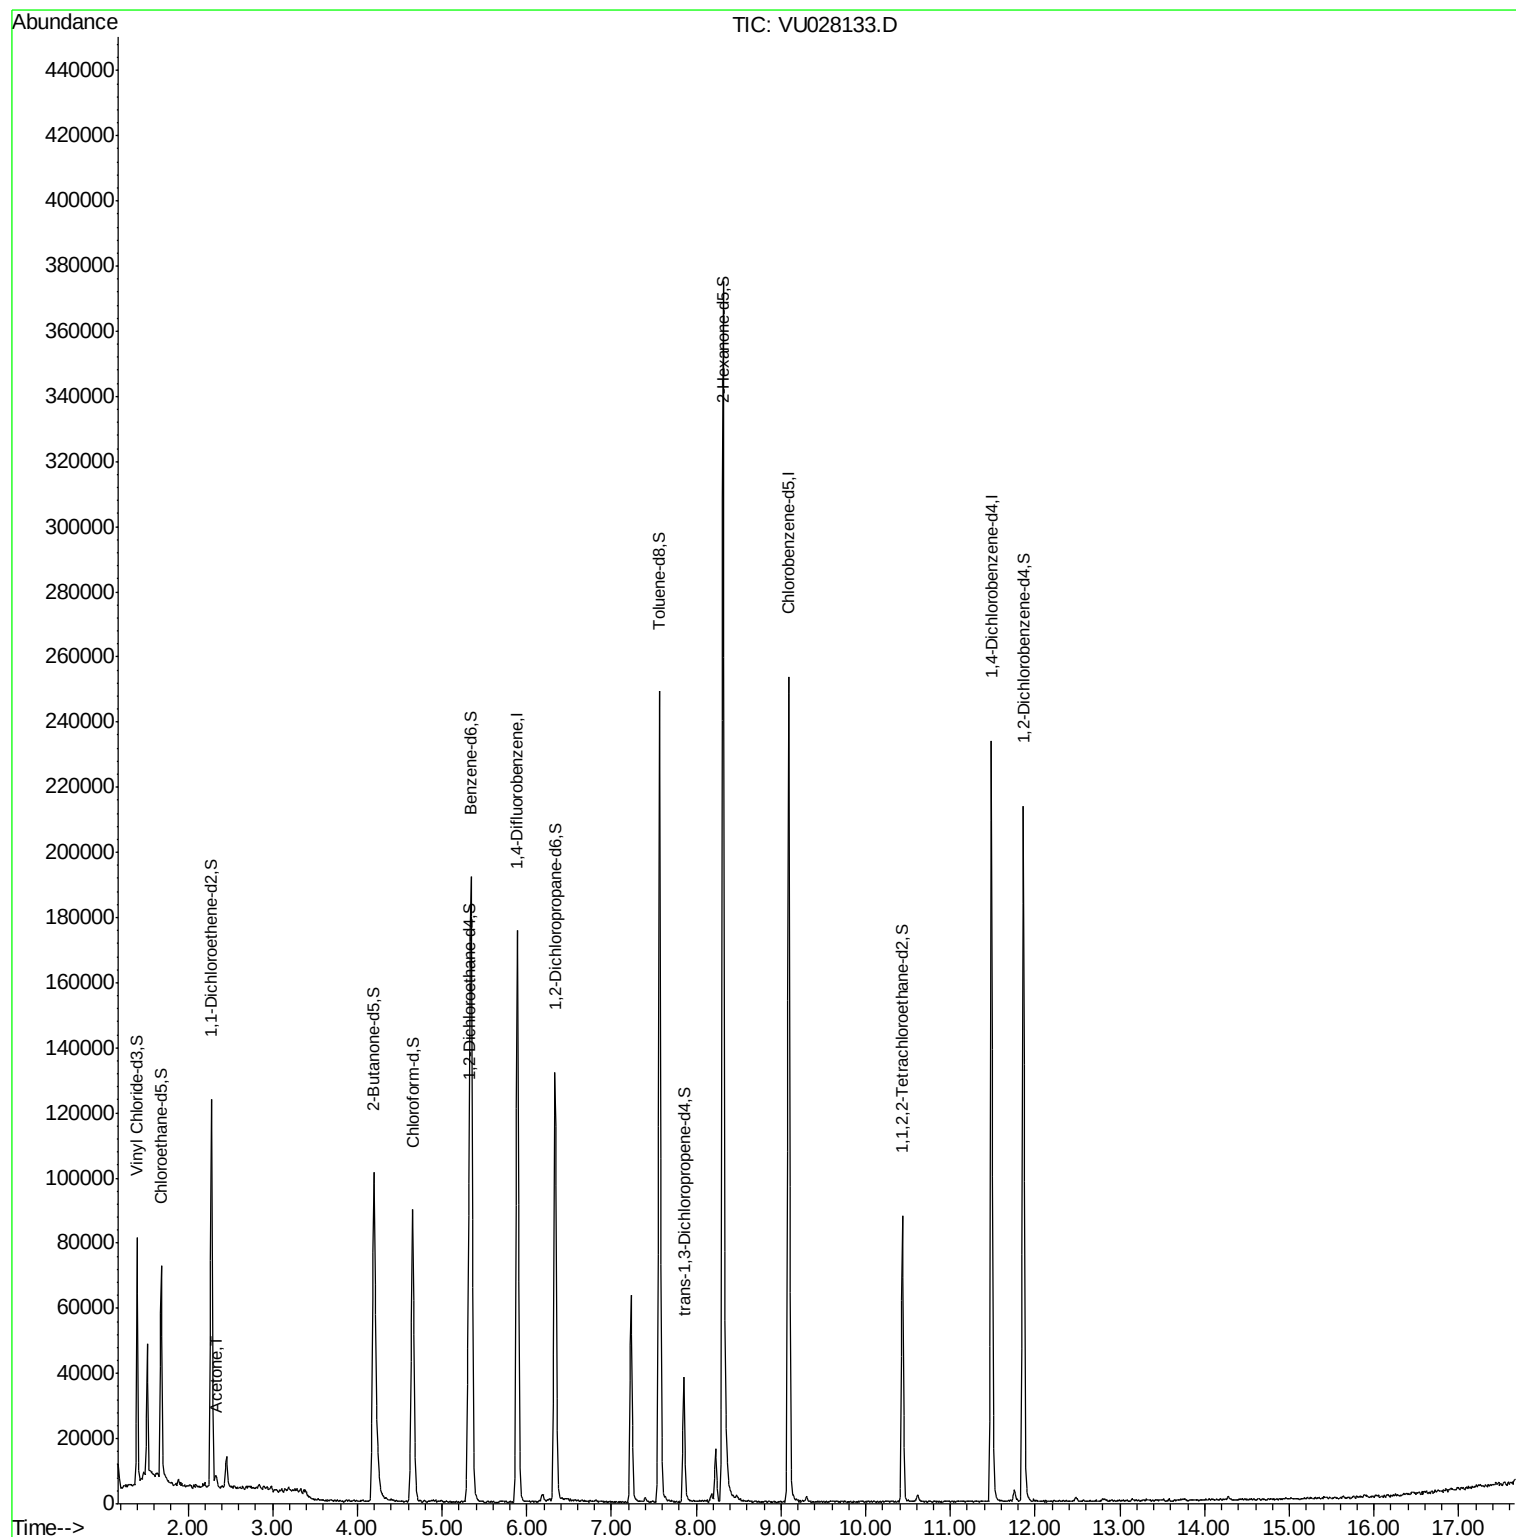

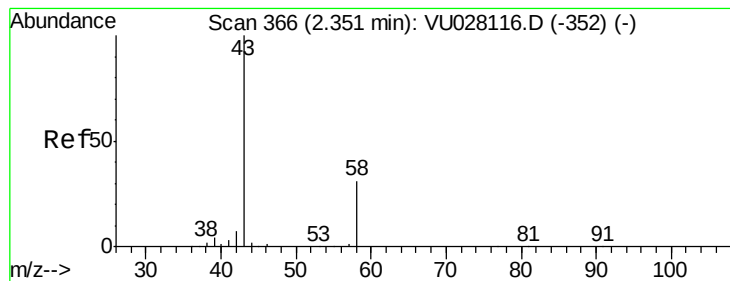

#13

Acetone

Concen: 1.254 ug/L

RT: 2.33 min Scan# 359

Delta R.T. -0.02 min

Lab File: VU028133.D

Acq: 14 Nov 2018 20:10

Instrument :

MSVOA_U

ClientSampleId :

F9C31

Tot Ion: 43 Resp: 2756

Ion Ratio Lower Upper

43 100

58 27.9 0.0 61.6

