

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111418\
 Data File : VU028135.D
 Acq On : 14 Nov 2018 20:57
 Operator : MD/SY
 Sample : J5948-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9C43

Quant Time: Nov 15 06:04:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 15 04:25:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	133483	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	126113	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	56808	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	49634	4.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.60%
7) Chloroethane-d5	1.68	69	40586	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.28	63	72007	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.19	46	164716	51.27	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.54%
24) Chloroform-d	4.65	84	85003	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	5.31	65	48814	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.34	84	175496	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	6.33	67	64678	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.57	98	154938	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	7.85	79	20152	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.31	63	128246	48.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	44347	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	52278	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	2522	1.166 ug/L	89
47) Tetrachloroethene	8.23	164	3064	0.359 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111418\
Data File : VU028135.D
Acq On : 14 Nov 2018 20:57
Operator : MD/SY
Sample : J5948-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9C43

Quant Time: Nov 15 06:04:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 15 04:25:02 2018
Response via : Initial Calibration

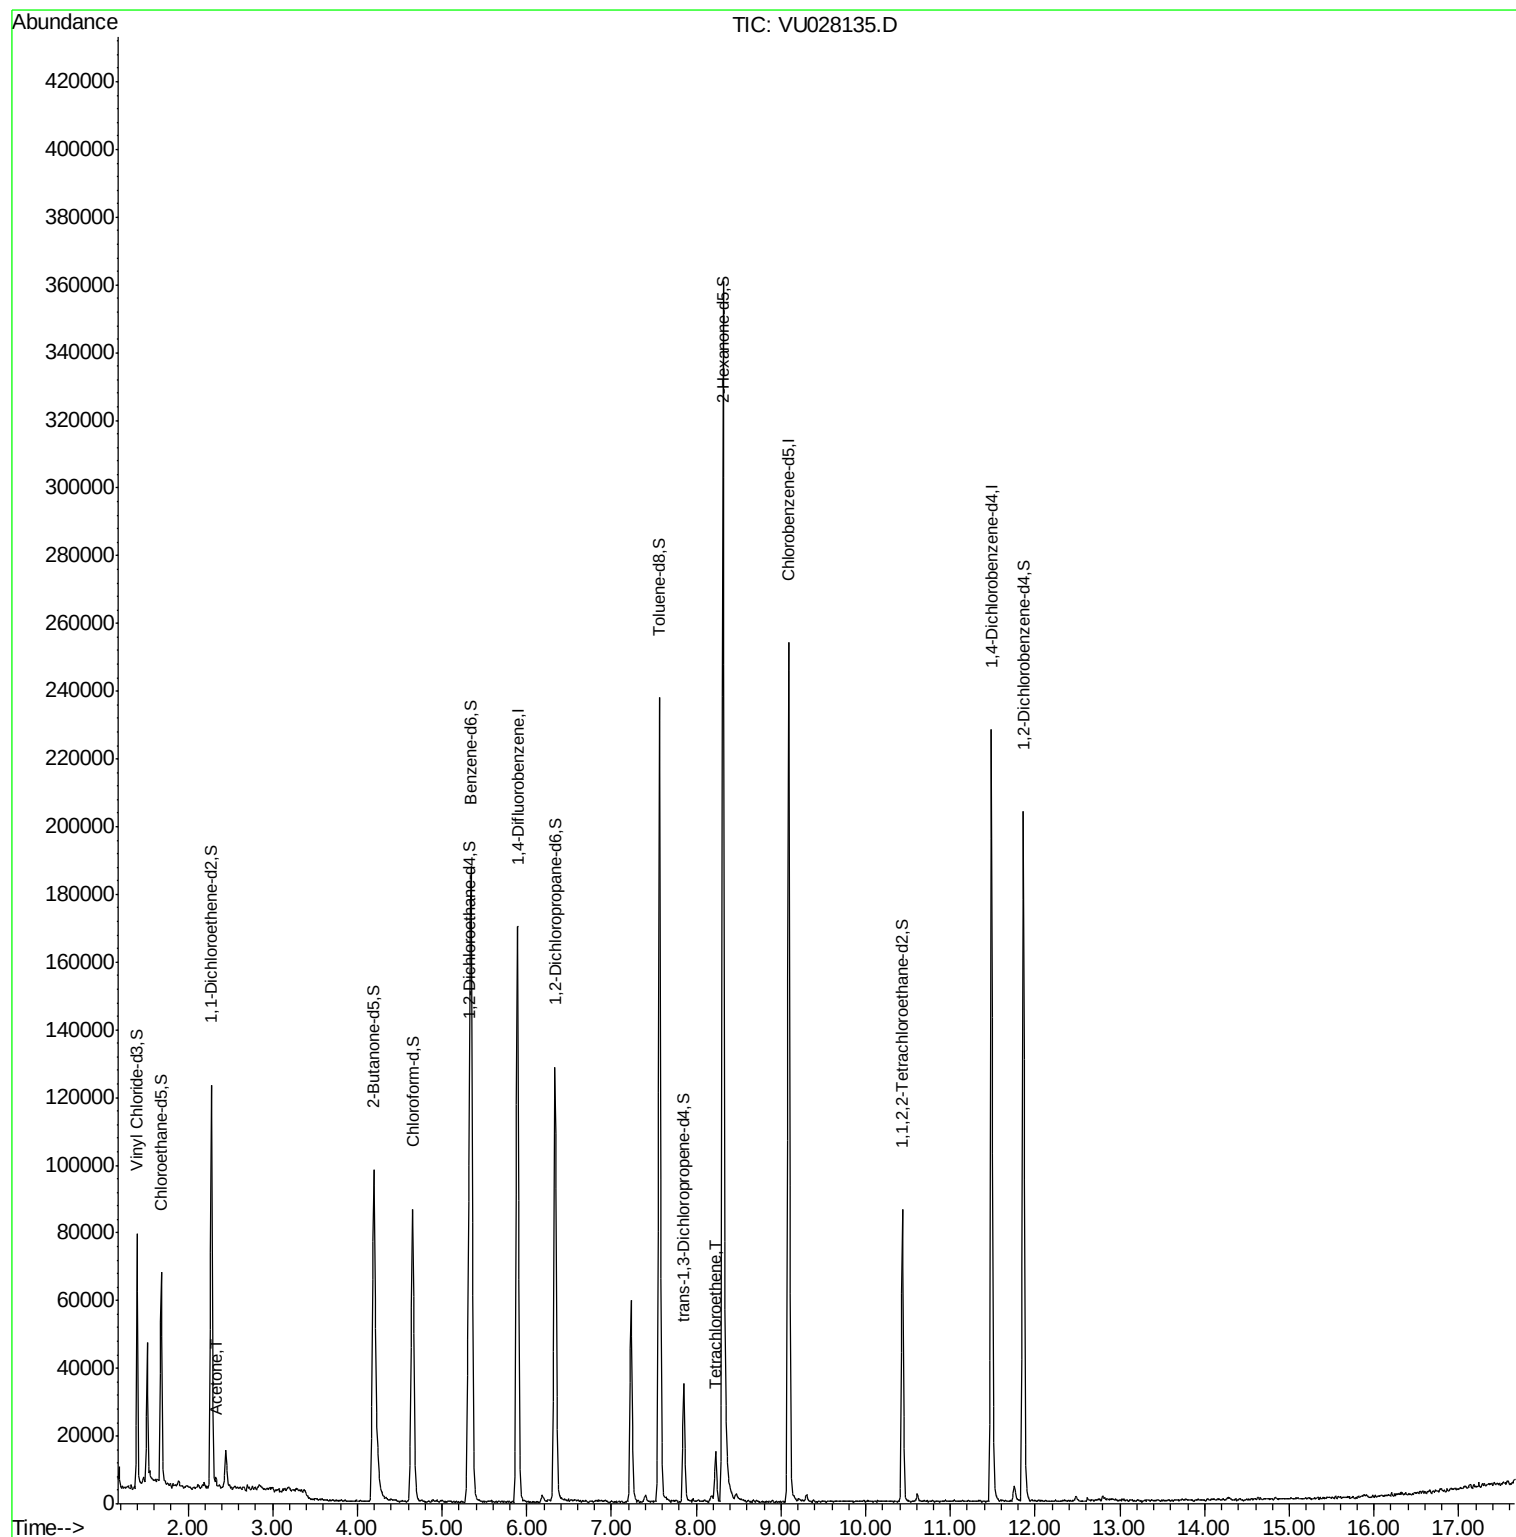

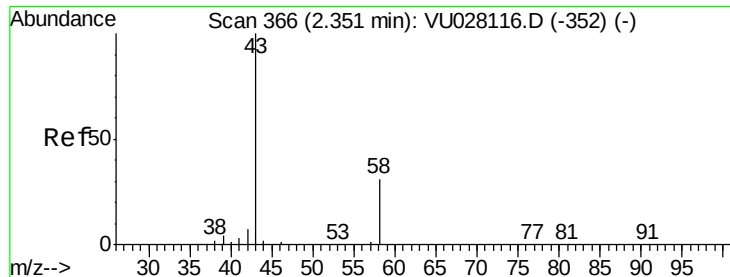

#13

Acetone

Concen: 1.166 ug/L

RT: 2.32 min Scan# 358

Delta R.T. -0.03 min

Lab File: VU028135.D

Acq: 14 Nov 2018 20:57

Instrument :

MSVOA_U

ClientSampleId :


F9C43

Tot Ion: 43 Resp: 2522

Ion Ratio Lower Upper




43 100

58 24.7 0.0 61.6

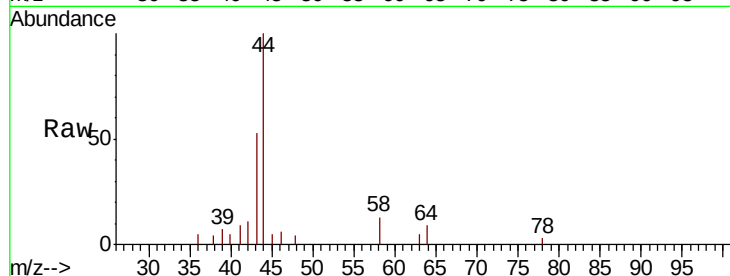

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

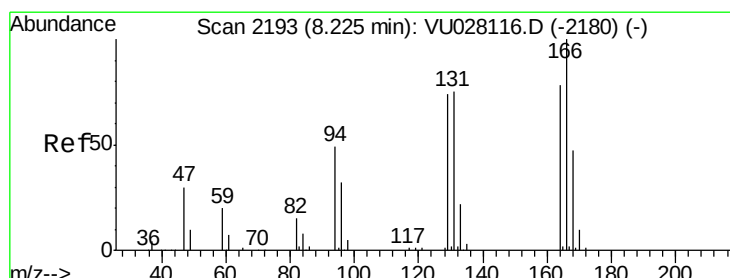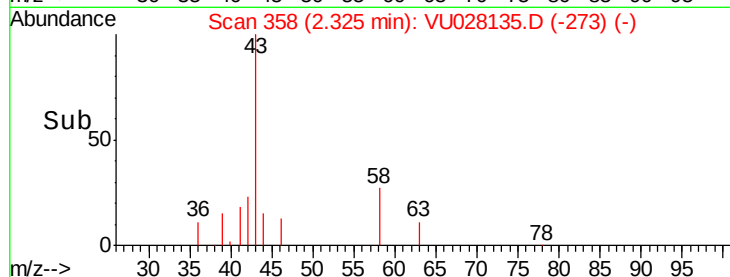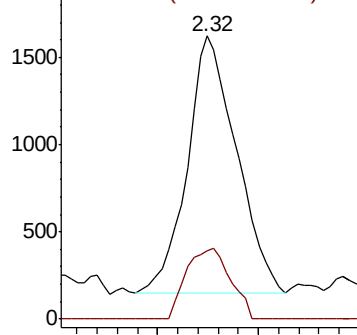

#47

Tetrachloroethene

Concen: 0.359 ug/L

RT: 8.23 min Scan# 2194

Delta R.T. 0.00 min

Lab File: VU028135.D

Acq: 14 Nov 2018 20:57

Tgt Ion:164 Resp: 3064


Ion Ratio Lower Upper

164 100

129 105.5 69.7 129.4

131 87.1 64.0 118.8

166 120.6 86.4 160.4

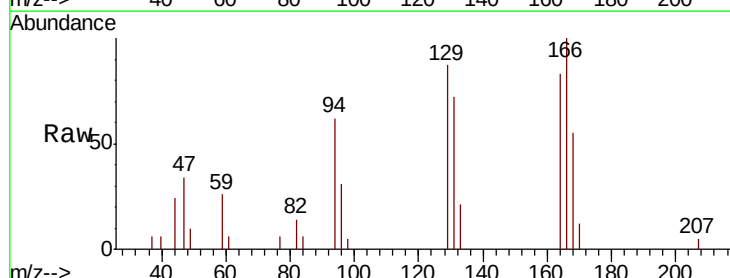

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

