


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111418\
Data File : VU028109.D
Acq On : 14 Nov 2018 09:26
Operator : MD/SY
Sample : BFB52
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Nov 15 06:14:20 2018

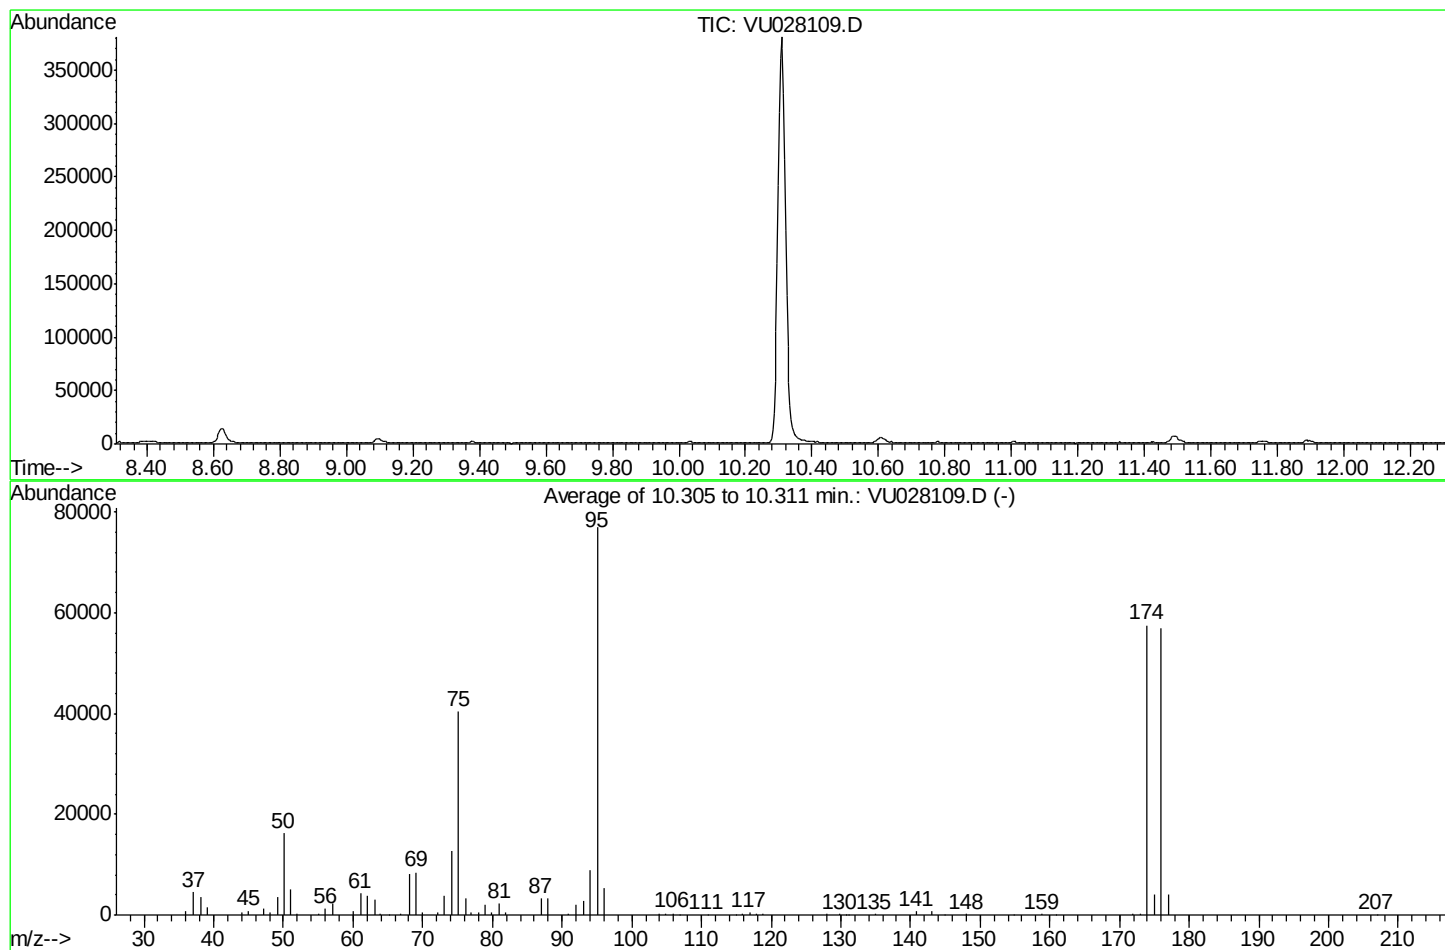

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	16256	PASS
75	95	30	80	52.4	40330	PASS
95	95	100	100	100.0	76976	PASS
96	95	5	9	6.8	5265	PASS
173	174	0.00	2	0.5	262	PASS
174	95	50	120	74.7	57469	PASS
175	174	5	9	7.1	4093	PASS
176	174	95	101	99.1	56957	PASS
177	176	5	9	7.1	4071	PASS

Scan 2828 (10.266 min): VU028109.D
BFB52

m/z	Abundance
39.90	206.0
43.00	171.0
44.00	537.0
45.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.10	847.0
37.10	4405.0
38.10	3824.0
39.10	1559.0
40.00	223.0
43.10	180.0
44.00	950.0
45.00	847.0
47.10	1160.0
48.10	480.0
49.10	3494.0
50.10	16245.0
51.10	5035.0
52.00	130.0
55.00	221.0
56.00	1117.0
57.10	2175.0
60.00	829.0
61.10	4264.0
62.10	3693.0
63.10	2860.0
63.90	227.0
65.10	102.0
66.90	222.0
68.10	7860.0
69.10	8271.0
70.00	564.0
72.10	510.0
73.10	3431.0
74.10	12748.0
75.10	39776.0
76.10	3459.0
77.00	555.0
78.00	467.0
79.00	1960.0
79.90	590.0
81.00	2204.0
81.90	498.0
87.00	3228.0
88.00	3424.0
91.10	215.0
92.10	2019.0
93.10	2793.0
94.10	8375.0
95.10	75576.0
96.10	5018.0
103.90	236.0
104.90	140.0
105.90	264.0
106.80	117.0
110.90	124.0
114.90	113.0
116.00	248.0
116.90	494.0
117.90	277.0
118.80	275.0
128.10	217.0
129.90	172.0
131.10	101.0
134.90	111.0
140.90	730.0
143.00	727.0
144.90	113.0
148.10	168.0
154.80	134.0
158.90	183.0
160.80	120.0
171.90	160.0
174.00	55120.0
175.00	4130.0
176.00	53928.0
177.00	3796.0
206.90	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	881.0
37.10	4690.0
38.10	3688.0
39.10	1603.0
40.00	198.0
43.10	174.0
44.00	959.0
45.00	895.0
47.10	1202.0
48.00	410.0
49.10	3610.0
50.10	16704.0
51.10	5278.0
52.00	198.0
55.10	257.0
56.00	1247.0
57.10	2315.0
60.00	817.0
61.00	4467.0
62.10	3937.0
63.10	3043.0
63.90	270.0
65.10	121.0
66.90	232.0
68.10	8523.0
69.10	8698.0
70.00	616.0
72.10	473.0
73.10	4014.0
74.10	13096.0
75.10	41800.0
76.10	3560.0
77.00	519.0
77.90	469.0
79.00	2149.0
79.90	593.0
81.00	2282.0
81.90	551.0
87.00	3371.0
88.00	3305.0
90.90	235.0
92.00	2108.0
93.10	2947.0
94.10	9078.0
95.10	79144.0
96.10	5418.0
103.90	260.0
104.80	160.0
105.90	331.0
106.90	131.0
115.90	276.0
116.90	515.0
117.90	277.0
118.80	329.0
127.90	235.0
129.90	250.0
134.90	155.0
140.90	787.0
143.00	795.0
148.00	140.0
154.80	100.0
158.90	212.0
171.90	158.0
174.00	58984.0
175.00	4126.0
176.00	58512.0
177.00	4258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.10	833.0
37.10	4333.0
38.10	3325.0
39.10	1485.0
39.90	177.0
43.10	151.0
44.00	990.0
45.00	888.0
47.10	1103.0
47.90	431.0
49.10	3435.0
50.10	15820.0
51.10	5028.0
52.00	225.0
55.10	236.0
56.00	1285.0
57.10	2185.0
60.00	809.0
61.00	4144.0
62.10	3748.0
63.10	2915.0
63.90	248.0
65.20	152.0
66.90	199.0
68.10	8423.0
69.10	8282.0
70.00	567.0
72.10	411.0
73.10	3925.0
74.10	12584.0
75.10	39416.0
76.10	3256.0
77.00	435.0
78.00	416.0
79.00	2165.0
79.90	580.0
81.00	2239.0
81.90	521.0
87.00	3231.0
88.00	2967.0
90.90	247.0
92.00	2097.0
93.10	2889.0
94.10	9007.0
95.10	76208.0
96.10	5359.0
104.00	281.0
104.80	151.0
105.90	317.0
106.90	101.0
115.90	278.0
116.90	467.0
118.00	231.0
118.80	373.0
127.80	255.0
129.90	298.0
130.80	101.0
134.90	167.0
140.90	766.0
143.00	746.0
148.00	114.0
158.90	153.0
171.90	116.0
173.00	786.0
174.00	58304.0
175.00	4025.0
176.00	58432.0
177.00	4161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52