


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111419\
 Data File : VU035706.D
 Acq On : 14 Nov 2019 08:48
 Operator : JC/SP
 Sample : BFB27
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 15 01:03:04 2019

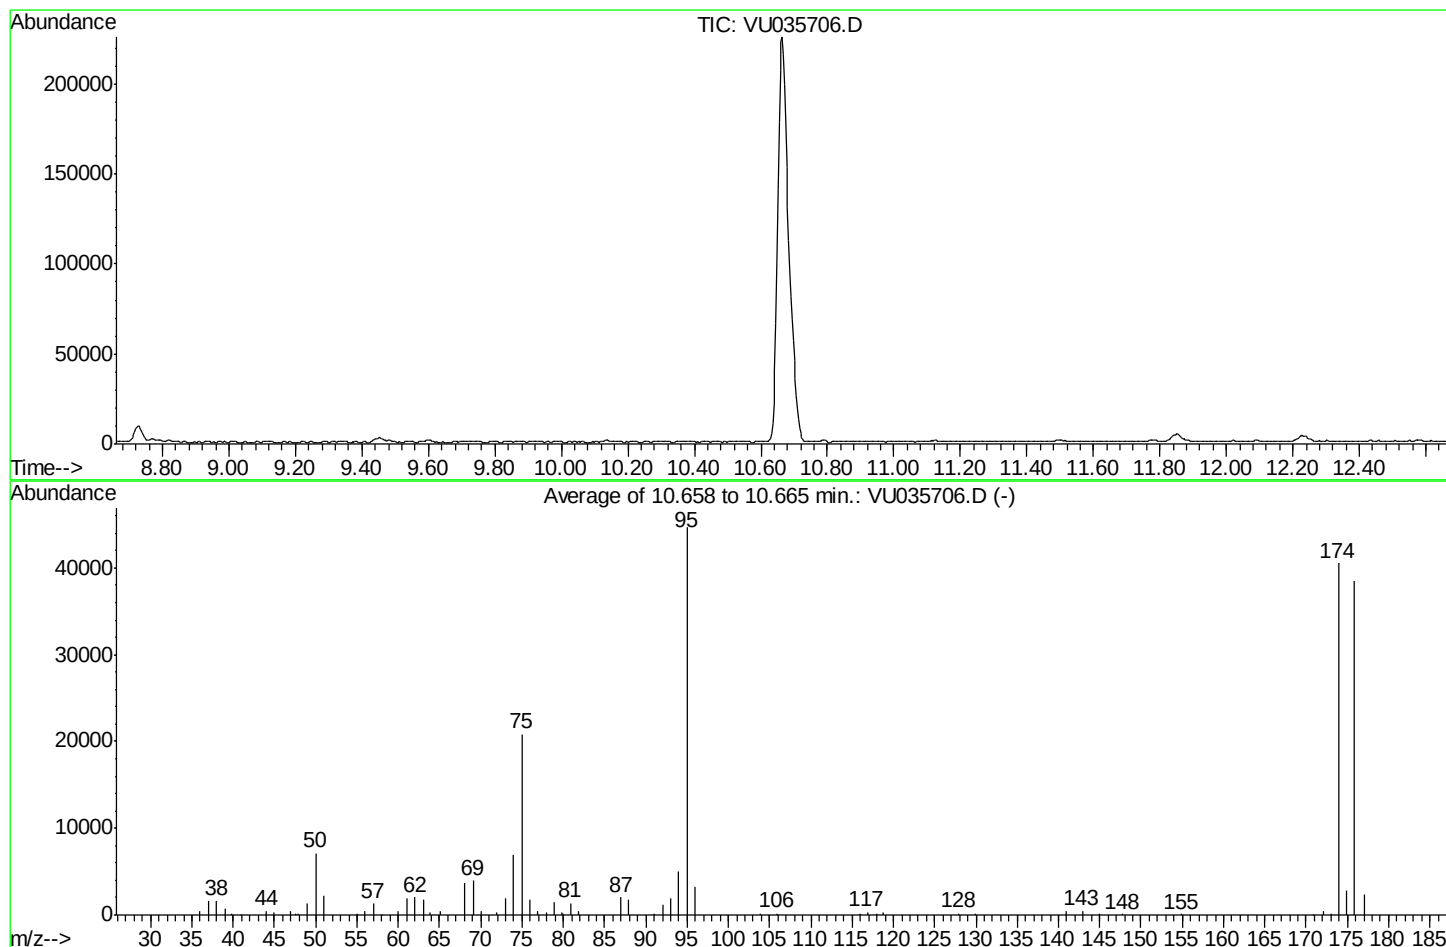

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	7154	PASS
75	95	30	80	46.7	20874	PASS
95	95	100	100	100.0	44672	PASS
96	95	5	9	7.3	3269	PASS
173	174	0.00	2	0.5	188	PASS
174	95	50	120	90.7	40496	PASS
175	174	5	9	7.1	2879	PASS
176	174	95	101	95.2	38562	PASS
177	176	5	9	6.2	2404	PASS

m/z	Abundance
35.90	409.0
37.00	1601.0
38.00	1672.0
39.00	669.0
39.90	329.0
40.90	103.0
44.00	1387.0
44.90	338.0
46.90	487.0
47.60	243.0
49.00	1322.0
50.00	7077.0
51.00	2171.0
55.10	100.0
55.90	475.0
57.00	1202.0
59.90	424.0
61.00	1881.0
62.00	1904.0
63.00	1749.0
63.90	233.0
65.10	352.0
68.00	3513.0
69.00	3858.0
70.00	352.0
72.00	287.0
73.00	1748.0
74.00	6647.0
75.00	19848.0
76.00	1724.0
76.90	309.0
77.90	340.0
79.00	1424.0
79.80	401.0
80.90	1239.0
81.90	350.0
87.00	1844.0
87.90	1789.0
90.90	155.0
92.00	1043.0
93.00	1715.0
94.00	4733.0
95.00	42968.0
96.00	3186.0
103.90	143.0
105.90	168.0
115.90	209.0
116.90	351.0
118.00	114.0
118.80	228.0
128.00	133.0
140.90	454.0
143.00	478.0
144.90	205.0
147.80	123.0
155.00	132.0
170.80	102.0
172.00	407.0
173.90	38008.0
174.90	2779.0
175.90	35856.0
177.00	2333.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	471.0
37.00	1630.0
38.00	1696.0
39.00	690.0
39.90	317.0
44.00	1423.0
44.90	329.0
46.90	501.0
47.60	258.0
49.00	1395.0
50.00	7309.0
51.00	2338.0
55.00	109.0
56.00	486.0
57.00	1357.0
60.00	394.0
61.00	2057.0
62.00	2100.0
63.00	1855.0
63.90	276.0
65.00	421.0
68.00	3732.0
69.00	3978.0
70.00	420.0
72.00	309.0
73.00	1844.0
74.00	7062.0
75.00	21200.0
76.00	1807.0
76.90	391.0
78.00	305.0
79.00	1575.0
79.80	380.0
80.90	1388.0
81.90	407.0
87.00	2032.0
87.90	1860.0
91.00	176.0
92.00	1165.0
93.00	2056.0
94.00	5060.0
95.00	45568.0
96.00	3368.0
103.90	156.0
105.90	179.0
115.90	198.0
116.80	382.0
117.90	170.0
118.80	360.0
127.90	158.0
129.90	125.0
140.90	472.0
142.90	447.0
144.90	240.0
147.80	142.0
154.90	142.0
172.10	463.0
173.90	41336.0
175.00	2930.0
175.90	39560.0
177.00	2467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	431.0
37.00	1584.0
38.00	1668.0
39.00	694.0
39.80	314.0
44.00	1440.0
45.00	349.0
46.90	480.0
47.90	299.0
49.00	1427.0
50.00	7078.0
51.00	2244.0
55.00	111.0
56.10	486.0
57.00	1265.0
58.00	110.0
60.00	348.0
61.00	2025.0
62.00	2079.0
63.00	1753.0
63.90	312.0
65.00	427.0
68.00	3886.0
69.10	4036.0
70.00	428.0
71.90	318.0
73.00	1964.0
74.00	7241.0
75.00	21576.0
76.00	1787.0
76.90	422.0
78.10	287.0
78.90	1618.0
80.00	411.0
80.90	1469.0
81.80	402.0
87.00	2127.0
87.90	1803.0
91.00	143.0
92.00	1208.0
93.10	2134.0
94.00	5133.0
95.00	45480.0
96.00	3254.0
103.90	176.0
105.90	175.0
115.90	157.0
116.80	352.0
117.90	232.0
118.80	409.0
127.90	186.0
129.90	178.0
141.00	404.0
142.90	461.0
144.90	219.0
147.80	123.0
154.90	131.0
172.10	494.0
173.00	566.0
173.90	42144.0
175.00	2928.0
175.90	40272.0
177.00	2413.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

Scan 2886 (10.620 min): VU035706.D
BFB27

m/z	Abundance
39.90	210.0
44.00	943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27