

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111423\
 Data File : VU056346.D
 Acq On : 15 Nov 2023 09:13
 Operator : MD/SY
 Sample : 05390-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0TN9

Quant Time: Nov 16 01:27:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 15 03:03:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	273357	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	274905	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	120066	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	55272	2.703	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	54.000%
7) Chloroethane-d5	1.911	69	53637	3.421	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.400%
11) 1,1-Dichloroethene-d2	2.563	65	28471	3.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	4.621	46	163827	40.183	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.360%
24) Chloroform-d	5.055	84	147484	3.729	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.600%
26) 1,2-Dichloroethane-d4	5.695	65	71333	3.903	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
32) Benzene-d6	5.721	84	278773	3.404	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.000%#
36) 1,2-Dichloropropane-d6	6.685	67	88447	3.583	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.600%
41) Toluene-d8	7.894	98	233469	3.228	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.600%#
43) trans-1,3-Dichloroprop...	8.177	79	31398	3.316	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.400%
46) 2-Hexanone-d5	8.627	63	131190	35.262	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.520%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	71802	4.071	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	86227	3.887	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	77.800%#
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	19434	5.597	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111423\
Data File : VU056346.D
Acq On : 15 Nov 2023 09:13
Operator : MD/SY
Sample : 05390-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0TN9


Quant Time: Nov 16 01:27:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 15 03:03:12 2023
Response via : Initial Calibration

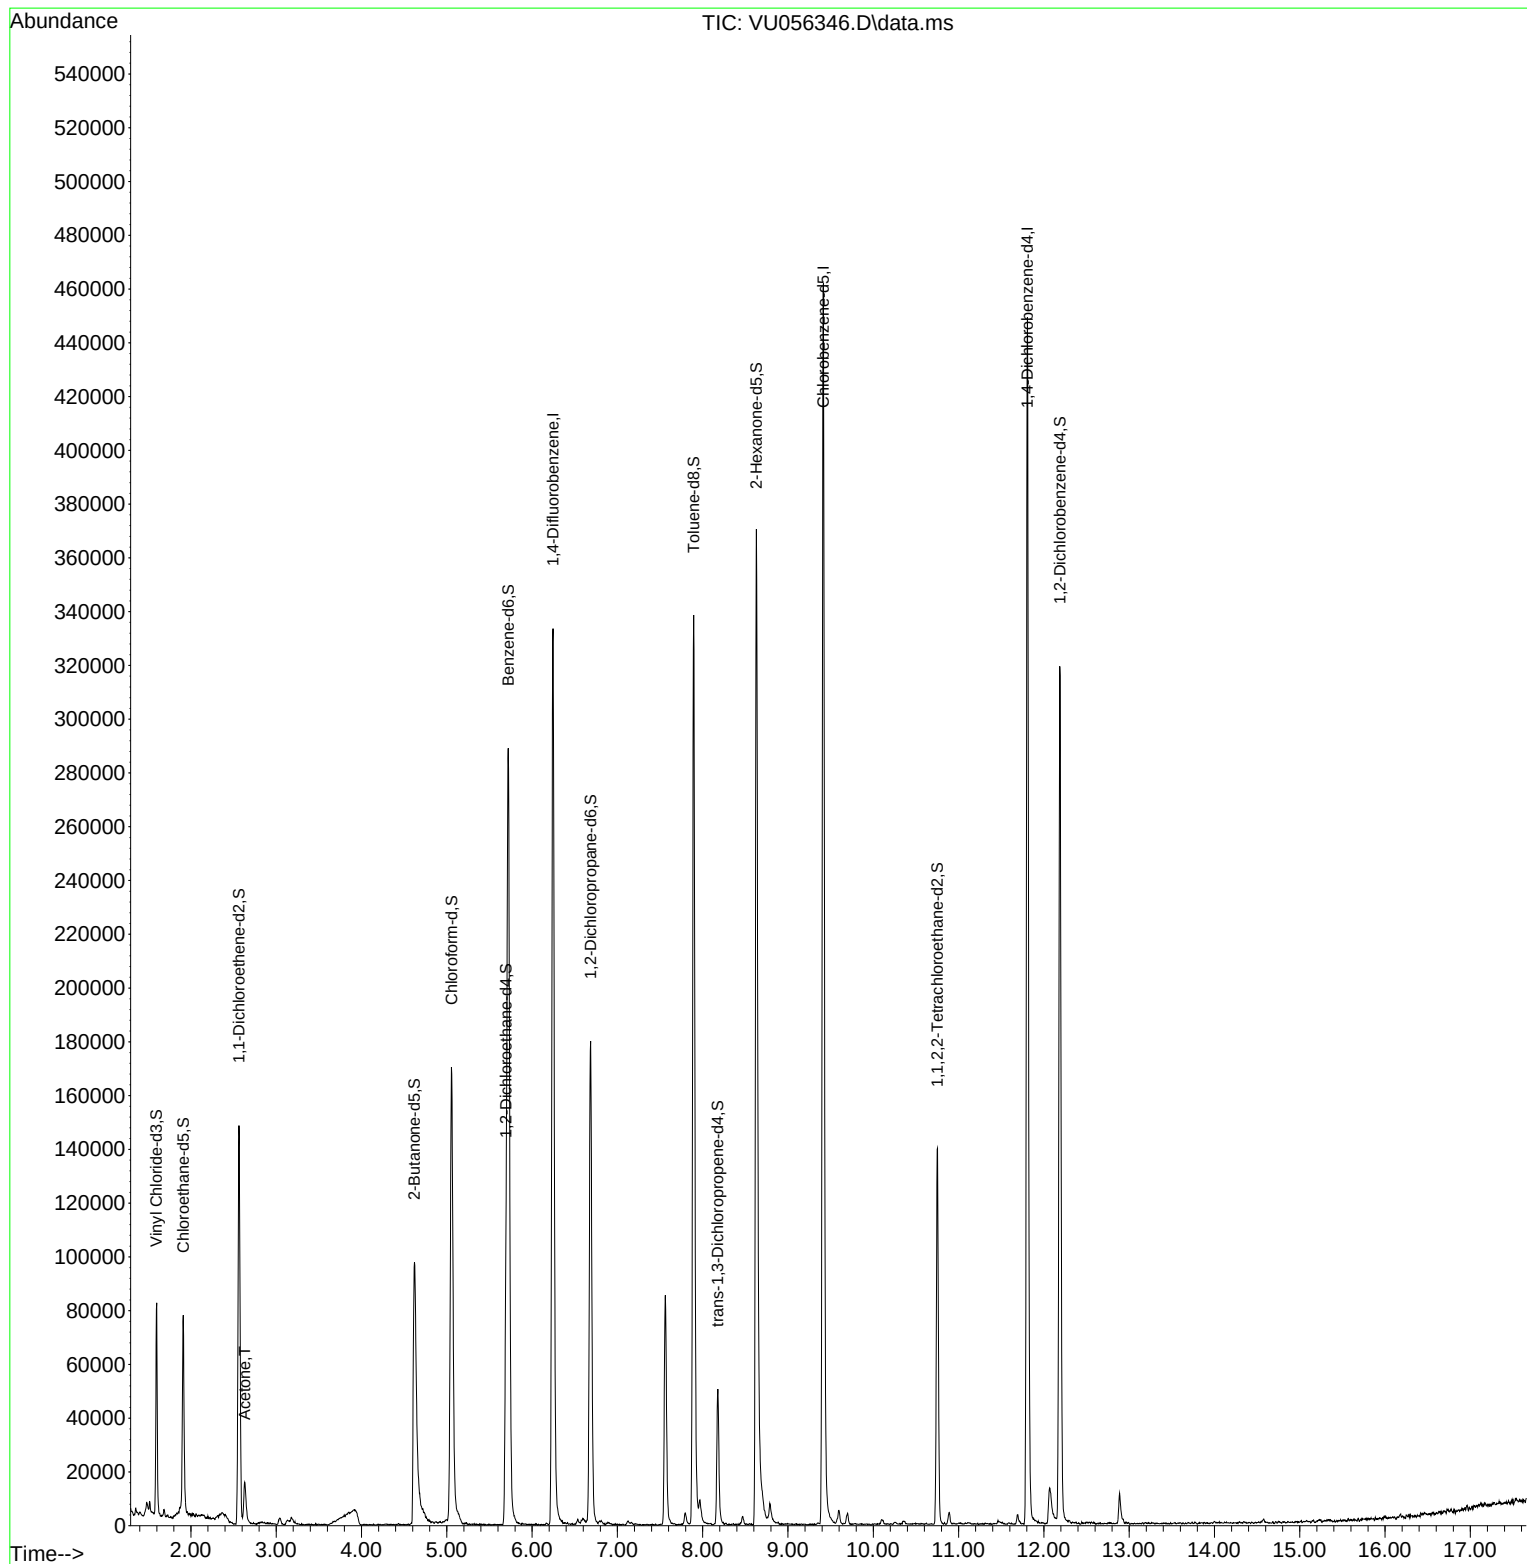

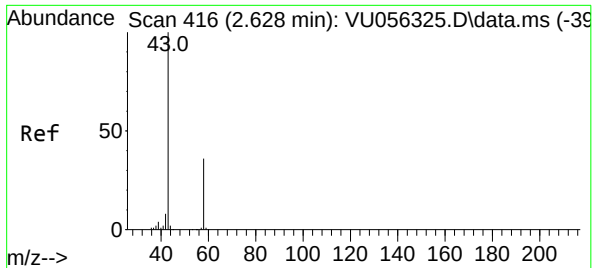

#13
 Acetone
 Concen: 5.597 ug/L
 RT: 2.631 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU056346.D
 Acq: 15 Nov 2023 09:13

Instrument :
 MSVOA_U
 ClientSampleId :
 C0TN9

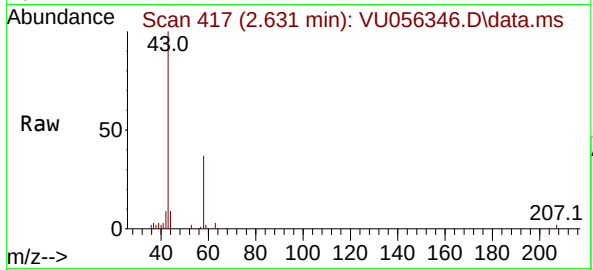

Tgt Ion: 43 Resp: 19434
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 70.0

