


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111423\
Data File : VU056324.D
Acq On : 14 Nov 2023 23:32
Operator : MD/SY
Sample : BFB073
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB073

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 17 04:03:21 2023

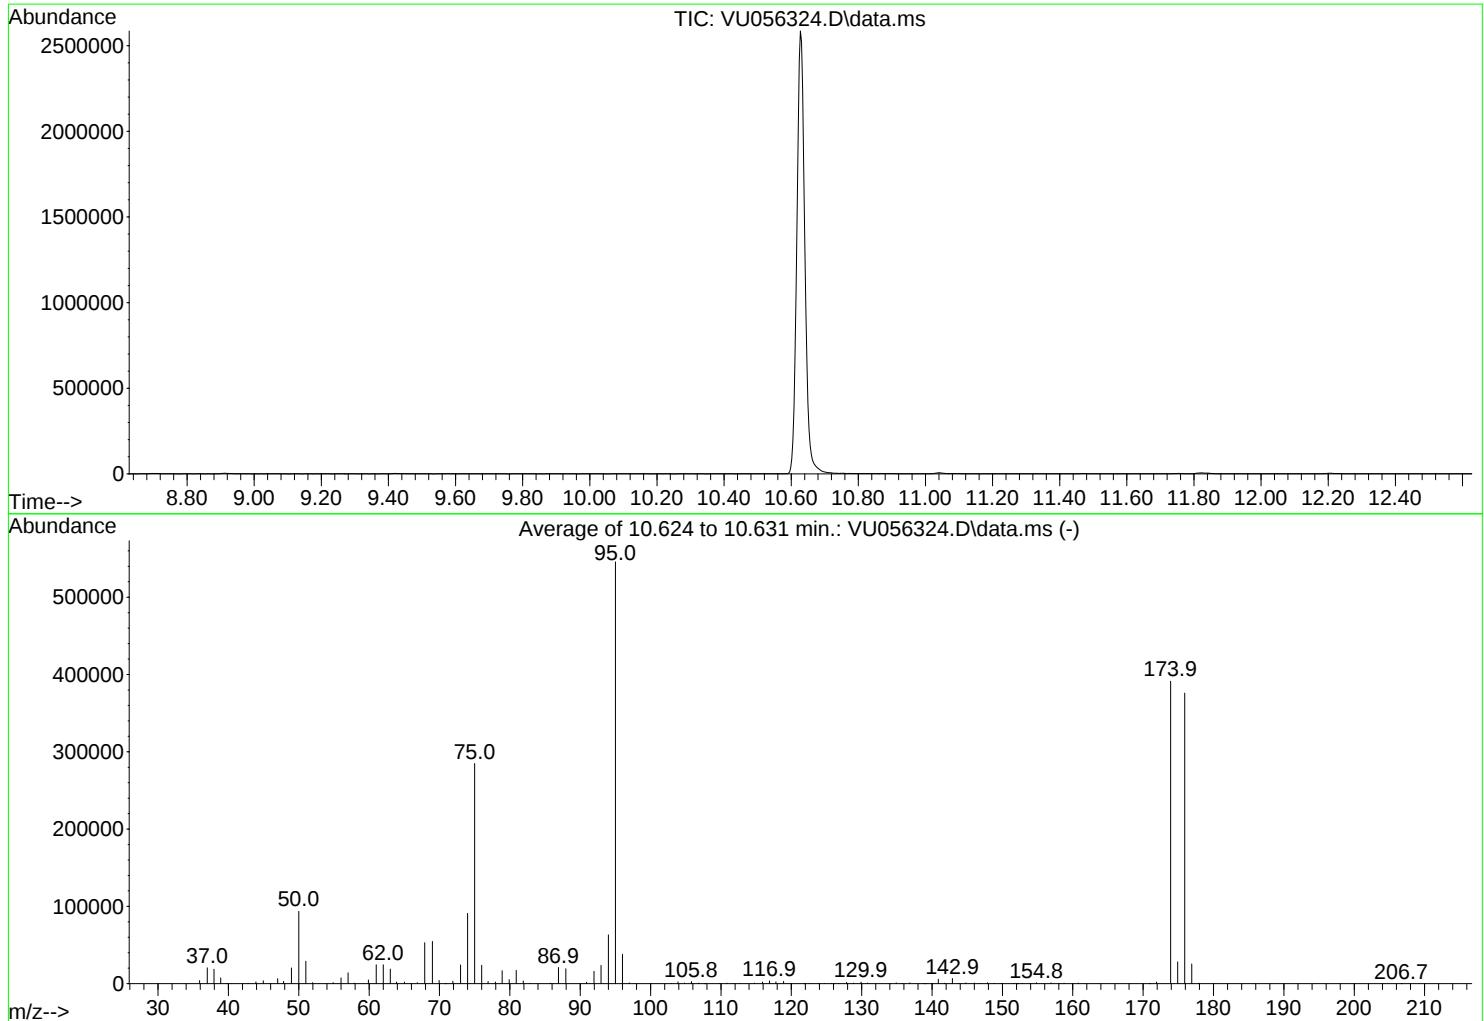

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	93643	PASS
75	95	30	80	52.2	284821	PASS
95	95	100	100	100.0	545771	PASS
96	95	5	9	6.9	37885	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.7	391317	PASS
175	174	5	9	7.2	28213	PASS
176	174	95	101	96.1	375957	PASS
177	176	5	9	6.8	25507	PASS

m/z	Abundance
40.00	136.0
43.80	531.0
77.10	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	4015.0
37.00	19712.0
38.00	18584.0
38.90	7426.0
39.80	559.0
40.50	208.0
42.80	170.0
43.90	2694.0
44.90	3533.0
46.00	415.0
47.00	6393.0
47.90	3001.0
49.00	20112.0
50.00	92160.0
51.00	28824.0
52.00	1323.0
52.90	316.0
54.90	1290.0
56.00	7211.0
57.00	13859.0
57.90	553.0
59.90	4675.0
61.00	23136.0
62.00	23608.0
63.00	18824.0
63.90	2160.0
65.00	2152.0
65.90	304.0
66.90	1303.0
67.90	52016.0
69.00	54248.0
70.00	3944.0
70.80	121.0
71.90	3141.0
73.00	24112.0
74.00	88856.0
75.00	276544.0
76.00	23288.0
76.90	2836.0
77.90	1932.0
78.90	16139.0
79.90	5201.0
80.90	16424.0
81.90	3501.0
82.90	414.0
85.80	579.0
86.90	20088.0
87.90	18928.0
90.90	1807.0
91.90	15749.0
92.90	23416.0
94.00	60712.0
95.00	526592.0
96.00	37376.0
96.90	965.0
103.00	285.0
103.90	2352.0
104.80	775.0
105.80	2750.0
106.90	608.0
107.70	121.0
109.90	248.0
110.90	470.0
111.80	250.0
112.70	516.0
114.70	787.0
115.90	1906.0
116.90	3358.0
117.80	2179.0
118.90	2762.0
121.80	136.0
122.70	163.0
123.90	464.0
124.70	199.0
126.00	153.0
126.70	171.0
127.90	1437.0
128.90	723.0
129.90	1905.0
130.90	863.0
134.00	141.0
134.90	1050.0
135.80	190.0
136.80	928.0
138.80	233.0
140.90	5342.0
141.70	485.0
142.90	6368.0
143.80	476.0
144.80	1149.0
146.00	768.0
146.80	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

147.90	1324.0
148.90	368.0
149.80	380.0
151.60	181.0
152.10	139.0
152.80	442.0
154.00	351.0
154.90	1201.0
155.90	196.0
156.90	882.0
158.00	170.0
158.70	535.0
160.80	505.0
170.90	265.0
171.90	2501.0
173.90	368768.0
174.90	27424.0
175.90	351488.0
176.90	24688.0
177.90	645.0
206.70	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	4203.0
37.00	21032.0
38.00	19264.0
38.90	7588.0
39.80	509.0
40.50	201.0
42.80	165.0
43.90	2860.0
44.90	3737.0
46.00	375.0
47.00	6619.0
47.80	3077.0
49.00	20760.0
50.00	96904.0
51.00	29720.0
52.00	1288.0
52.90	302.0
54.90	1291.0
56.00	7760.0
57.00	14569.0
57.90	561.0
59.90	4958.0
61.00	25096.0
62.00	25152.0
63.00	19496.0
63.90	2018.0
65.00	2035.0
65.90	259.0
66.90	1393.0
67.90	54880.0
69.00	56672.0
69.90	4212.0
70.80	135.0
71.90	3156.0
73.00	24800.0
74.00	93752.0
75.00	293376.0
76.00	24600.0
76.90	3237.0
78.00	2065.0
78.90	17336.0
79.90	5394.0
80.90	17848.0
81.90	3665.0
82.90	444.0
85.80	530.0
86.90	21480.0
88.00	19752.0
90.90	2035.0
91.90	16488.0
92.90	24264.0
94.00	64976.0
95.00	563456.0
96.00	39008.0
97.00	981.0
102.90	286.0
103.90	2458.0
104.80	750.0
105.80	2853.0
106.80	586.0
107.70	105.0
109.80	248.0
110.80	620.0
111.80	263.0
112.70	502.0
114.80	847.0
115.90	2169.0
116.90	3621.0
117.80	2396.0
118.90	2858.0
121.80	123.0
122.60	234.0
123.90	435.0
124.70	209.0
125.70	176.0
126.80	154.0
127.80	1573.0
128.80	827.0
129.90	2131.0
130.80	976.0
134.00	172.0
134.90	1099.0
135.70	182.0
136.90	1038.0
138.70	191.0
140.90	5866.0
141.70	566.0
142.90	6942.0
143.80	480.0
144.80	1162.0
146.00	862.0
146.80	326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

147.90	1371.0
148.90	426.0
149.90	446.0
151.70	237.0
152.10	186.0
152.80	473.0
154.00	292.0
154.90	1385.0
155.90	298.0
156.90	1091.0
158.00	207.0
158.80	576.0
160.80	605.0
171.90	2216.0
173.90	403968.0
174.90	29168.0
175.90	387584.0
176.90	26384.0
177.90	729.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	3900.0
37.00	20568.0
37.90	18072.0
38.90	7256.0
39.80	462.0
42.80	154.0
44.00	3015.0
45.00	3780.0
45.90	277.0
47.00	6171.0
47.80	2914.0
48.90	19848.0
50.00	91864.0
51.00	28296.0
51.90	1139.0
52.70	291.0
54.90	1197.0
56.00	7497.0
57.00	13611.0
57.90	524.0
59.90	4718.0
61.00	24904.0
62.00	24648.0
63.00	18232.0
63.90	1939.0
65.00	1829.0
66.00	205.0
66.80	1366.0
67.90	52144.0
69.00	53208.0
69.90	4087.0
70.80	100.0
71.90	2822.0
73.00	23776.0
74.00	90392.0
75.00	284544.0
76.00	23464.0
76.90	3335.0
78.00	2138.0
78.90	16984.0
79.90	5130.0
80.90	17360.0
81.90	3638.0
82.80	464.0
85.80	543.0
86.90	21048.0
88.00	19216.0
90.90	1984.0
92.00	15603.0
93.00	23160.0
94.00	63776.0
95.00	547264.0
96.00	37272.0
97.00	1011.0
102.90	269.0
103.90	2370.0
104.80	727.0
105.80	2529.0
106.80	570.0
109.70	267.0
110.80	732.0
111.80	276.0
112.70	448.0
114.80	723.0
115.90	2243.0
116.90	3534.0
117.80	2360.0
118.90	2829.0
119.90	148.0
122.60	231.0
123.90	323.0
124.70	151.0
125.70	237.0
126.80	134.0
127.80	1694.0
128.80	939.0
129.90	2077.0
130.80	983.0
134.10	182.0
134.90	1011.0
135.70	217.0
136.90	1071.0
138.70	111.0
139.00	115.0
139.90	366.0
140.90	6029.0
141.80	601.0
142.90	6765.0
143.80	402.0
144.80	1063.0
146.00	757.0
146.80	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

147.90	1305.0
148.80	406.0
149.90	519.0
151.70	278.0
152.80	408.0
153.90	302.0
154.80	1510.0
155.90	336.0
156.90	1147.0
158.10	213.0
158.80	641.0
160.80	676.0
171.90	1819.0
173.90	401216.0
174.90	28048.0
175.90	388800.0
176.90	25448.0
177.90	816.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073