


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111518\
Data File : VU028159.D
Acq On : 15 Nov 2018 08:17
Operator : MD/SY
Sample : BFB53
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB53

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 16 00:43:47 2018

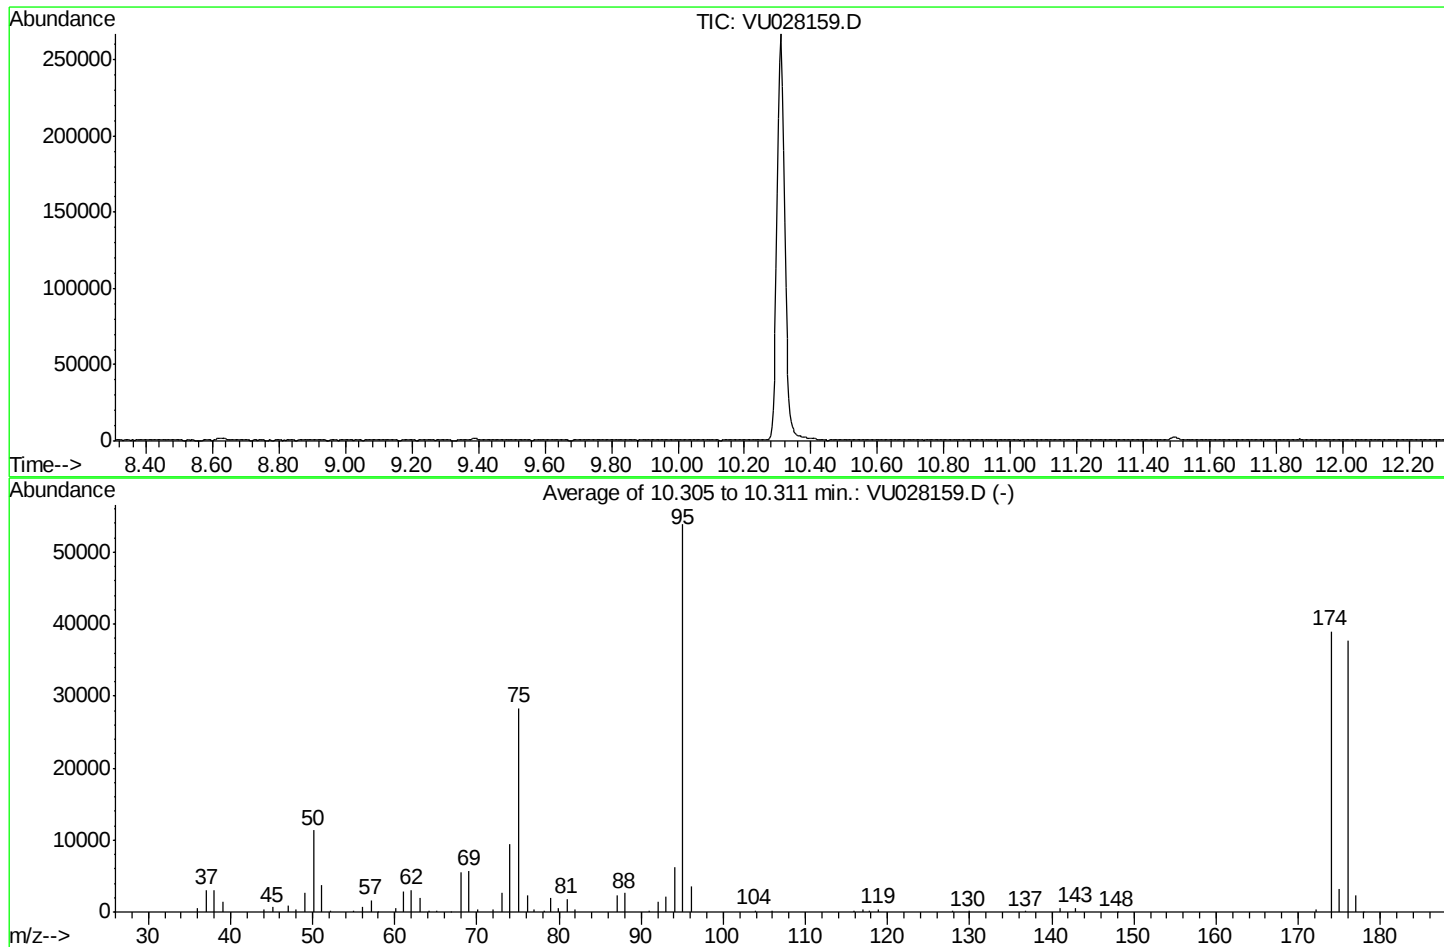

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	11325	PASS
75	95	30	80	52.5	28272	PASS
95	95	100	100	100.0	53850	PASS
96	95	5	9	6.8	3645	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	38968	PASS
175	174	5	9	8.2	3209	PASS
176	174	95	101	96.8	37712	PASS
177	176	5	9	6.4	2404	PASS

Scan 2828 (10.266 min): VU028159.D
BFB53

m/z	Abundance
39.90	176.0
44.10	527.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	573.0
37.10	3060.0
38.10	2851.0
39.10	1407.0
44.00	704.0
45.10	661.0
47.10	1000.0
47.90	270.0
49.00	2539.0
50.10	10838.0
51.10	3626.0
52.10	187.0
55.00	118.0
56.00	716.0
57.10	1634.0
58.00	129.0
60.10	668.0
61.10	2931.0
62.00	2963.0
63.10	1880.0
64.10	186.0
65.00	155.0
66.90	159.0
68.10	5633.0
69.10	5816.0
70.00	438.0
72.00	371.0
73.10	2640.0
74.00	9518.0
75.10	28504.0
76.10	2379.0
77.00	309.0
78.10	187.0
79.00	2064.0
79.90	535.0
81.00	1773.0
81.90	346.0
87.00	2422.0
88.00	2663.0
91.00	217.0
92.00	1386.0
93.00	2109.0
94.10	6388.0
95.10	55016.0
96.10	3670.0
103.90	317.0
105.90	293.0
115.90	242.0
116.90	277.0
117.80	224.0
118.90	426.0
127.80	139.0
129.90	180.0
136.80	101.0
141.00	539.0
142.90	527.0
172.10	298.0
174.00	39592.0
175.00	3266.0
176.00	38552.0
177.00	2427.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	544.0
37.10	3097.0
38.00	2990.0
39.10	1357.0
40.00	134.0
44.00	913.0
45.10	614.0
47.10	775.0
48.00	339.0
49.10	2686.0
50.10	11493.0
51.10	3760.0
52.20	229.0
55.00	164.0
56.00	838.0
57.10	1587.0
60.00	521.0
61.10	2695.0
62.10	3070.0
63.10	1913.0
64.10	283.0
65.10	167.0
68.10	5376.0
69.00	5498.0
70.10	408.0
72.00	358.0
73.00	2487.0
74.10	9197.0
75.10	27112.0
76.10	2391.0
77.00	258.0
78.20	224.0
79.00	1791.0
79.90	496.0
81.00	1747.0
81.90	370.0
87.00	2195.0
88.00	2489.0
91.00	248.0
92.00	1435.0
93.00	2080.0
94.10	6025.0
95.10	50872.0
96.10	3601.0
103.90	200.0
105.90	201.0
115.90	230.0
117.10	368.0
117.80	218.0
118.90	281.0
127.90	159.0
129.90	180.0
136.80	104.0
141.00	540.0
142.90	588.0
148.00	117.0
172.10	304.0
174.00	37176.0
175.00	3039.0
176.00	35744.0
177.00	2315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	571.0
37.10	3186.0
38.10	3077.0
39.10	1480.0
44.00	790.0
45.10	676.0
47.10	938.0
47.90	314.0
49.00	2705.0
50.10	11646.0
51.10	3954.0
52.20	240.0
55.00	156.0
56.00	816.0
57.10	1721.0
58.00	144.0
60.10	628.0
61.10	2943.0
62.00	3154.0
63.10	1959.0
64.10	242.0
65.00	166.0
66.80	126.0
68.10	5753.0
69.10	5891.0
70.00	432.0
72.00	396.0
73.00	2687.0
74.00	9806.0
75.10	29200.0
76.10	2438.0
77.00	278.0
78.20	223.0
79.00	2038.0
79.90	547.0
81.00	1853.0
81.90	369.0
87.00	2450.0
88.00	2710.0
91.00	250.0
92.00	1456.0
93.00	2190.0
94.10	6527.0
95.10	55664.0
96.10	3665.0
103.90	265.0
105.90	263.0
115.90	280.0
117.00	306.0
117.90	224.0
118.90	386.0
127.90	171.0
129.90	169.0
136.80	122.0
141.00	534.0
142.90	597.0
148.00	119.0
172.10	313.0
174.00	40136.0
175.00	3323.0
176.00	38840.0
177.00	2470.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53