

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111519\
 Data File : VU035726.D
 Acq On : 15 Nov 2019 15:04
 Operator : JC/SP
 Sample : K5759-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2J21

Quant Time: Nov 16 02:36:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 16 01:36:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	209029	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	239188	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	90130	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	82050	3.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.20%
7) Chloroethane-d5	1.93	69	78777	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.60%
11) 1,1-Dichloroethene-d2	2.59	63	107910	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	4.70	46	246681	51.93	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.86%
24) Chloroform-d	5.11	84	166414	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	5.75	65	88107	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.77	84	310808	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.60%
36) 1,2-Dichloropropane-d6	6.74	67	109576	4.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.00%
41) Toluene-d8	7.93	98	244536	3.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.60%#
43) trans-1,3-Dichloropropene-	8.21	79	37516	3.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.20%
46) 2-Hexanone-d5	8.69	63	159951	41.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.96%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	96140	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	86251	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
13) Acetone	2.67	43	25188	7.354 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111519\
Data File : VU035726.D
Acq On : 15 Nov 2019 15:04
Operator : JC/SP
Sample : K5759-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2J21

Quant Time: Nov 16 02:36:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 16 01:36:54 2019
Response via : Initial Calibration

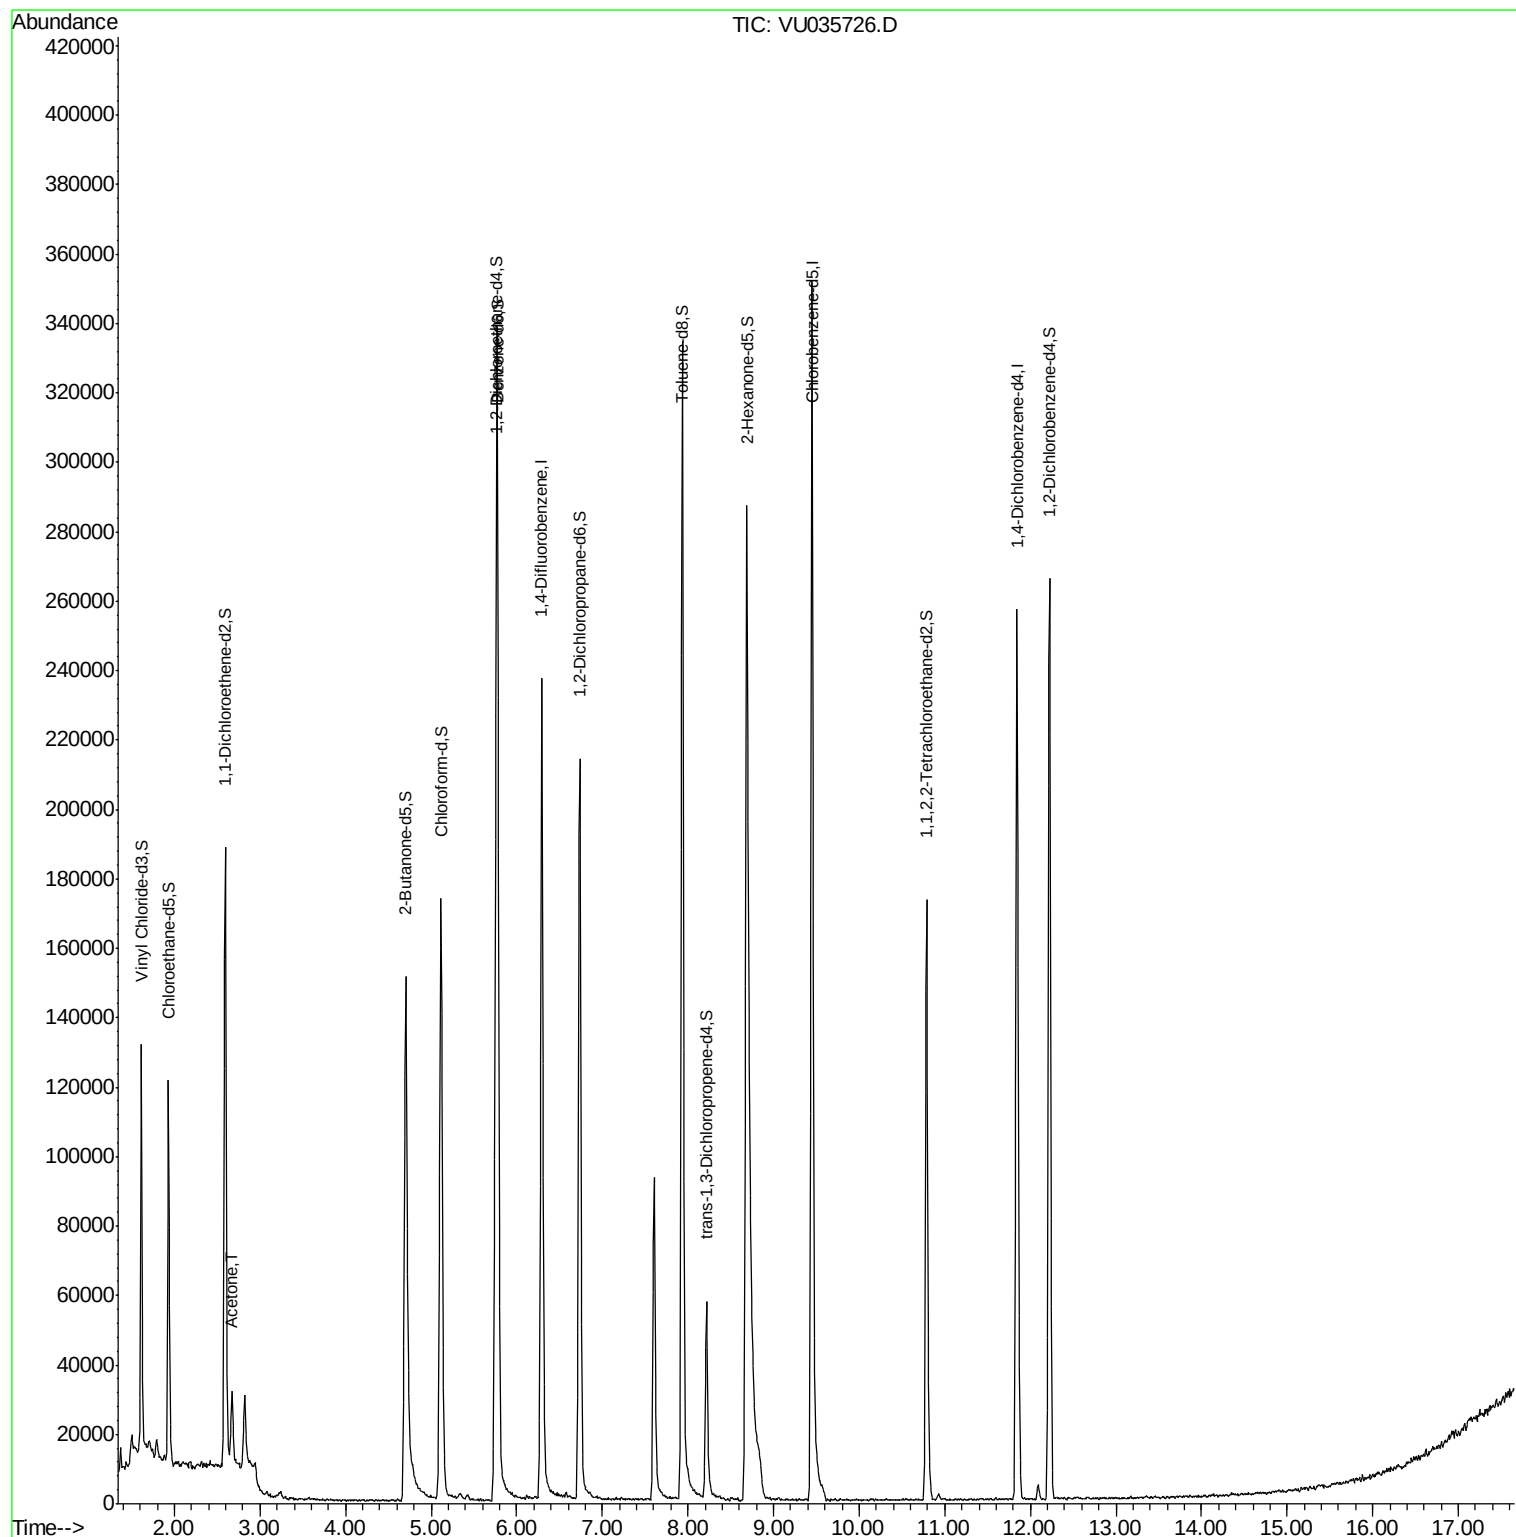

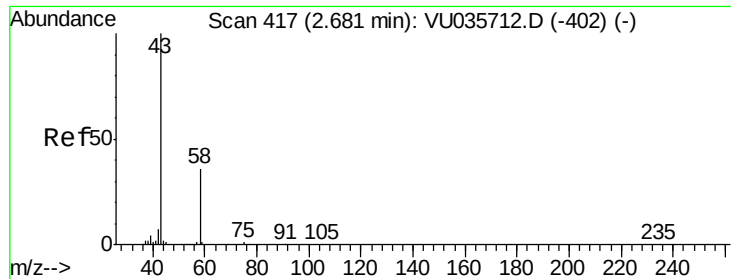

#13
 Acetone
 Concen: 7.354 ug/L
 RT: 2.67 min Scan# 415
 Delta R.T. -0.01 min
 Lab File: VU035726.D
 Acq: 15 Nov 2019 15:04

Instrument :
 MSVOA_U
 ClientSampleId :
 F2J21

Tot Ion: 43 Resp: 25188
 Ion Ratio Lower Upper
 43 100
 58 36.6 0.0 69.8

